

# User Manual



## Thermohygrometer Indicator

with NIST-Traceable Calibration

### Model 20250-30



THE STANDARD IN PRECISION MEASUREMENT

## **Introduction**

The Digi-Sense Thermohygrometer Indicator (Model 20250-30) is designed for indoor applications, and displays temperature, humidity, and time. Advanced features include °C/°F unit selection, Max/Min reading for temperature and humidity, environmental comfort indicators, and clock with alarm and date. The instrument is fully tested and calibrated to NIST-traceable standards. Careful use of this meter will provide years of reliable service.

## **Unpacking**

Check individual parts against the list of items below. If anything is missing or damaged, please contact your instrument supplier immediately.


1. Indicator
2. One AAA (1.5 V) battery, installed
3. C-clip for mounting
4. User manual
5. NIST-traceable calibration report with data

## Key Features

- User-selectable °C or °F units
- Built-in sensor for indoor temperature and humidity measurement
- Max/Min temperature and humidity displays
- Environmental symbols displayed: COMFORT (comfortable), WET (high humidity), DRY (low humidity)
- Clock with alarm and date

## Meter Description

1. LCD (three readouts)
2. **MODE** button
3. **ADJ** adjustment button
4. **MEMO** memory button
5. °C/°F button (on back of unit)
6. **RESET** button (on back of unit)

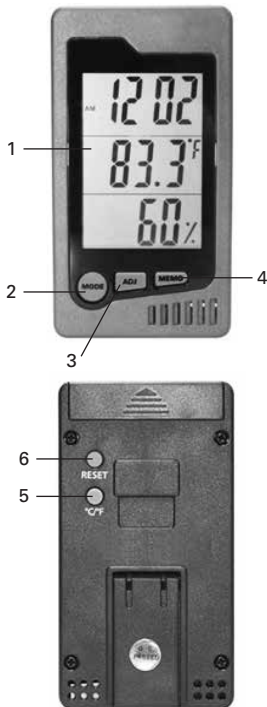

# Setup and Operation

## Button Functions

1. **MODE** switches from clock to alarm function
2. **ADJ** sets clock, alarm, and date
3. **MEMO** displays Max/Min temperature and humidity readings
4. **°C/°F** changes temperature display unit of measure
5. **RESET** clears all settings and memory data

## Display

1. The screen is divided into three parts:
  - a. Section one displays time, date, and alarm
  - b. Section two displays temperature readings (in either °C or °F)
  - c. Section three displays relative humidity % and comfort indicator symbols

## View Current Time and Date

1. Press the **ADJ** button to toggle between viewing time and date.

## View Max/Min Temperature and Humidity

1. Press the **MEMO** button to toggle between Current/Max/Min/Current.
2. Press the **MEMO** button for longer than two seconds to clear the Max/Min memory.

## Environmental Comfort Display Symbols

1. Temperature at 68 to 78.8°F (20 to 26°C) and relative humidity between 50% and 70% RH will show 😊 **COMFORT** symbol.
2. Any temperature and relative humidity above 70% RH shows the 😓 **WET** symbol for high humidity.
3. Any temperature and relative humidity below 50% RH shows 😞 **DRY** symbol for low humidity.

## Setting Clock and Date

1. Press **MODE** button to make sure you are in the time mode and not alarm mode. Once in time mode, press and hold the **MODE** button for three seconds to activate.
2. The *minutes* will start to blink; use the **ADJ** button to increase value (see Fig. 1).
3. Press **MODE** button to advance to *hours* and use the **ADJ** button to change to desired setting.
4. Press **MODE** button to advance to *12- or 24-hour* mode and use the **ADJ** button to change value (see Fig. 2).
5. Press **MODE** button to advance to *month* and use the **ADJ** button to change to desired setting (see Fig. 3).
6. Press **MODE** button to advance to *date* and use the **ADJ** button to change to desired setting (see Fig. 3).




Fig. 1




Fig. 2




Fig. 3

## Setup and Operation (continued)

### Setting Alarm

1. Press **MODE** button to make sure you are in the alarm mode and not the time mode. Once in alarm mode, press and hold the **MODE** button for three seconds to activate.
2. The *minutes* will start to blink; use the **ADJ** button to change to desired setting (see Fig. 4).
3. Press the **MODE** button to advance to *hours* and use the **ADJ** button to change to desired setting.






Fig. 4

### Activating the Alarm

1. Press the **MODE** button to advance to turning the alarm on/off hours and use the **ADJ** button to change the value (see Fig. 5).
  - a.  symbol indicates alarm is active in chime mode.
  - b.  symbol indicates the alarm is active in sound mode.




Fig. 5

2. Press the **MODE** button to exit.

### Changing Unit of Measure

1. Temperature unit displayed can be changed from °C to °F by pressing the °C/°F button on the back of the unit.

### Reset Button

1. Press and hold **RESET** button on the back of the unit to clear all information and default to the factory settings.

## **Specifications**

<b>Range</b>	
Humidity	10 to 90% RH
Temperature	32 to 120°F (0 to 50°C)
<b>Resolution</b>	
Humidity	1%
Temperature	0.1°F/C
<b>Accuracy</b>	
Humidity	±5% (40% RH ~ 80% RH), ±8% remaining range
Temperature	±1.8°F (1°C) 32 to 120°F (0 to 50°C)

Display	LCD
Auto power-off	Unit shuts off automatically after six minutes to preserve battery life
Weight	3 oz (85 g)
Dimensions (L x W x H)	4¼" x 2¼" x 5/16" (10.8 x 5.7 x 0.8 cm)
Power	One AAA battery

## **Maintenance, Recalibration, and Repair**

### **Cleaning and Storage**

- Meter should be cleaned with a damp cloth and mild detergent when necessary. Do not use solvents or abrasives.
- Store meter in an area with moderate temperature and humidity.

### **Battery Replacement**

If the battery power is insufficient, open the battery cover on the back of the unit and replace the AAA battery. Close the cover securely.

## **Maintenance, Recalibration, and Repair (cont.)**

**It is recommended that Digi-Sense products are calibrated annually** to ensure proper function and accurate measurements; however, your quality system or regulatory body may require more frequent calibrations.

## **For Product and Ordering Information, Contact:**

Contact:  
Industrial Process Measurement, Inc.  
3910 Park Avenue, Unit 7  
Edison, NJ 08820  
732-632-6400  
support@instrumentation2000.com  
<http://www.instrumentation2000.com>