Arbitrary Function Generator

AFG-2225

User Manual

GW INSTEK PART NO.82AF-22250EA1

ISO-9001 CERTIFIED MANUFACTURER

GW INSTEK

This manual contains proprietary information, which is protected by copyright. All rights are reserved. No part of this manual may be photocopied, reproduced or translated to another language without prior written consent of Good Will Corporation.

The information in this manual was correct at the time of printing. However, Good Will continues to improve its products and therefore reserves the right to change the specifications, equipment, and maintenance procedures at any time without notice.

Good Will Instrument Co., Ltd.
No. 7-1, Jhongsing Rd., Tucheng Dist., New Taipei City 236, Taiwan.

Table of Contents

SAFETY INSTRUCTIONS 6

GETTING STARTED 11
Main Features 11
Panel Overview 13
Setting Up the function Generator 19

QUICK REFERENCE 21
How to use the Digital Inputs 23
How to use the Help Menu 25
Selecting a Waveform 27
Modulation 29
Sweep 34
Burst 35
ARB 37
Utility Menu 40
Frequency Counter 41
Coupling 42
Menu Tree 44
Default Settings 52

OPERATION 54
Select a Waveform 55

MODULATION 64
Amplitude Modulation (AM) 66
Frequency Modulation (FM) 75
Frequency Shift Keying (FSK) Modulation 84
Phase Modulation (PM) 91
SUM modulation 100
Frequency Sweep 108

Burst Mode 118

SECONDARY SYSTEM FUNCTION SETTINGS 131
Save and Recall 132
System and Settings 136
System and Settings 136

CHANNEL SETTINGS 143

ARBITRARY WAVEFORMS 147
Inserting Built-In Waveforms 148
Display an Arbitrary Waveform 150
Editing an Arbitrary Wavefrom 159
Ouput an Arbitrary Waveform 169
Saving/Loading an Arbitrary Waveform 171

REMOTE INTERFACE 180
Establishing a Remote Connection 181
Command List 189
System Commands 193
Status Register Commands 196
System Remote Commands 199
Apply Commands 200
Output Commands 206
Pulse Configuration Commands 216
Amplitude Modulation (AM) Commands 218
AM Overview 218
Frequency Modulation (FM) Commands 223
FM Overview 223
Frequency-Shift Keying (FSK) Commands 228
FSK Overview 228
Phase Modulation (PM)Commands 232
PM Overview 232

SUM Modulation (SUM) Commands 236
SUM Overview 236
Frequency Sweep Commands 240
Sweep Overview 240
Burst Mode Commands 249
Burst Mode Overview 249
Arbitrary Waveform Commands 260
Arbitrary Waveform Overview 260
COUNTER 266
PHASE 267
COUPLE 268
Save and Recall Commands 271
Error Messages 273
SCPI Status Register 281

APPENDIX 287
AFG-2225 Specifications 287
EC Declaration of Conformity 292

INDEX 305

SAFETY INSTRUCTIONS

This chapter contains important safety instructions that should be followed when operating and storing the function generator. Read the following before any operation to ensure your safety and to keep the function generator in the best condition.

Safety Symbols

These safety symbols may appear in this manual or on the instrument.

WARNING	Warning: Identifies conditions or practices that could result in injury or loss of life.
CAUTION	Caution: Identifies conditions or practices that could result in damage to the function generator or to other objects or property.
	DANGER High Voltage
	Attention: Refer to the Manual
	Protective Conductor Terminal
	Earth (Ground) Terminal
	DANGER Hot Surface

Double Insulated

Do not dispose electronic equipment as unsorted municipal waste. Please use a separate collection facility or contact the supplier from which this instrument was purchased.

Safety Guidelines

General Guideline CAUTION	• Do not place heavy objects on the instrument. • Do not place flammable objects on the instrument. • Avoid severe impact or rough handling that may damage the function generator. • Avoid discharges of static electricity on or near the function generator. • Use only mating connectors, not bare wires, for the terminals. • The instrument should only be disassembled by a qualified technician. (Measurement categories) EN 61010-1:2010 specifies the measurement categories and their requirements as follows. The AFG-2225 falls under category II. • Measurement category IV is for measurement performed at the source of a low-voltage installation. • Measurement category III is for measurement performed in a building installation. • Measurement category II is for measurement performed on circuits directly connected to a low voltage installation. • Measurement category I is for measurements performed on circuits not directly connected to Mains.
Power Supply WARNING	• AC Input voltage: 100 ~ 240V AC, 50 ~ 60Hz. • Connect the protective grounding conductor of the AC power cord to an earth ground to prevent electric shock.

Fuse ⚠ WARNING	• Fuse type: F1A/250V. • Only qualified technicians should replace the fuse. • To ensure fire protection, replace the fuse only with the specified type and rating. • Disconnect the power cord and all test leads before replacing the fuse. • Make sure the cause of fuse blowout is fixed before replacing the fuse.
Cleaning the function generator	• Disconnect the power cord before cleaning the function generator. • Use a soft cloth dampened in a solution of mild detergent and water. Do not spray any liquid into the function generator. • Do not use chemicals containing harsh products such as benzene, toluene, xylene, and acetone.
Operation Environment	• Location: Indoor, no direct sunlight, dust free, almost non-conductive pollution (Note below) and avoid strong magnetic fields. • Relative Humidity: < 80% • Altitude: < 2000m • Temperature: 0°C to 40°C

	(Pollution Degree) EN 61010-1:2010specifies pollution degrees and their requirements as follows. The function generator falls under degree 2. Pollution refers to “addition of foreign matter, solid, liquid, or gaseous (ionized gases), that may produce a reduction of dielectric strength or surface resistivity”. • Pollution degree 1: No pollution or only dry, non-conductive pollution occurs. The pollution has no influence. • Pollution degree 2: Normally only non-conductive pollution occurs. Occasionally, however, a temporary conductivity caused by condensation must be expected. • Pollution degree 3: Conductive pollution occurs, or dry, non-conductive pollution occurs which becomes conductive due to condensation which is expected. In such conditions, equipment is normally protected against exposure to direct sunlight, precipitation, and full wind pressure, but neither temperature nor humidity is controlled.
Storage environment	• Location: Indoor • Relative Humidity: < 70% • Temperature: -10°C to 70°C
Disposal	Do not dispose this instrument as unsorted municipal waste. Please use a separate collection facility or contact the supplier from which this instrument was purchased. Please make sure discarded electrical waste is properly recycled to reduce environmental impact.

Power cord for the United Kingdom

When using the function generator in the United Kingdom, make sure the power cord meets the following safety instructions.

NOTE: This lead/appliance must only be wired by competent persons

⚠ WARNING: THIS APPLIANCE MUST BE EARTHED

IMPORTANT: The wires in this lead are coloured in accordance with the following code:

Green/ Yellow:	Earth
Blue:	Neutral
Brown:	Live (Phase)

As the colours of the wires in main leads may not correspond with the coloured marking identified in your plug/appliance, proceed as follows:

The wire which is coloured Green & Yellow must be connected to the Earth terminal marked with either the letter E, the earth symbol ⏚ or coloured Green/Green & Yellow.

The wire which is coloured Blue must be connected to the terminal which is marked with the letter N or coloured Blue or Black.

The wire which is coloured Brown must be connected to the terminal marked with the letter L or P or coloured Brown or Red.

If in doubt, consult the instructions provided with the equipment or contact the supplier.

This cable/appliance should be protected by a suitably rated and approved HBC mains fuse: refer to the rating information on the equipment and/or user instructions for details. As a guide, a cable of 0.75mm^2 should be protected by a 3A or 5A fuse. Larger conductors would normally require 13A types, depending on the connection method used.

Any exposed wiring from a cable, plug or connection that is engaged in a live socket is extremely hazardous. If a cable or plug is deemed hazardous, turn off the mains power and remove the cable, any fuses and fuse assemblies. All hazardous wiring must be immediately destroyed and replaced in accordance to the above standard.

GETTING STARTED

The Getting started chapter introduces the function generator's main features, appearance, set up procedure and power-up.

Main Features

Model name	Frequency bandwidth
AFG-2225	25MHz
Performance	• DDS Function Generator series • 1μHz high frequency resolution maintained at full range • 20ppm frequency stability • Arbitrary Waveform Capability 120 MSa/s sample rate 60 MSa/s repetition rate 4k-point waveform length 10 groups of 4k waveform memories True waveform output to display User-defined output section DWR (Direct Waveform Reconstruction) capability Waveform editing via PC
Features	• Sine, Square, Ramp, Pulse, Noise, standard waveforms • Internal and external LIN/LOG sweep with marker output

	• Int/Ext AM, FM, PM, FSK, SUM modulation • Burst function with internal and external triggers without marker output • Store/recall 10 groups of setting memories • Output overload protection
Interface	• USB interface as standard • 3.5 inch Color TFT LCD (320 X 240) graphical user interface • AWES (Arbitrary Waveform Editing Software) PC software

Panel Overview

Front Panel

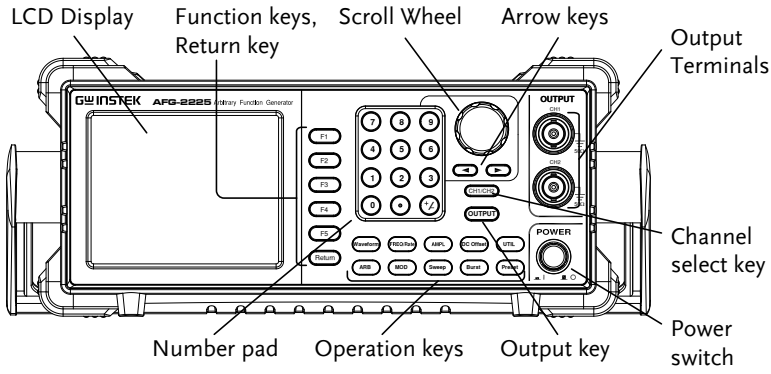

LCD Display	TFT color display, 320 x 240 resolution.	
Function Keys F1~F5	F1	Activates functions which appear on the right-hand side of the LCD display.
Return Key	Return	Goes back to the previous menu level.
Operation Keys	Waveform	The waveform key is used to select a type of waveform.
	FREQ/Rate	The FREQ/Rate key is used to set the frequency or sample rate.
	AMP	AMPL sets the waveform amplitude.
	DC Offset	Sets the DC offset.

		The UTIL key is used to access the save and recall options, update and view the firmware version, access the calibration options, output impedance settings and frequency meter.
		ARB is used to set the arbitrary waveform parameters.
		The MOD, Sweep and Burst keys are used to set the modulation, sweep and burst settings and parameters.
Preset Key		The preset key is used to recall a preset state.
Output Key		The Output key is used to turn on or off the waveform output.
Channel Select Key		The channel select key is used to switch between the two output channels.
Output ports		CH1: Channel 1 output port CH2: Channel 2 output port
Power Button		Turns the power on or off.
Arrow Keys		Used to select digits when editing parameters.

Scroll Wheel		The scroll wheel is used to edit values and parameters.  Decrease Increase
Keypad		The digital keypad is used to enter values and parameters. The keypad is often used in conjunction with the arrow keys and variable knob.

Rear Panel

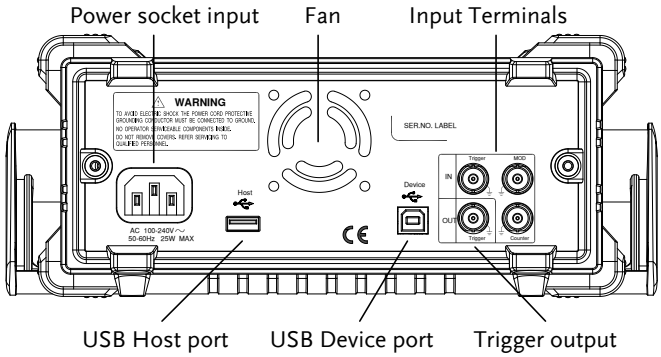

Trigger Input		External trigger input. Used to receive external trigger signals.
Trigger Output		Marker output signal. Used for Sweep and ARB mode only.
Fan		Fan.
Power Input Socket		Power input: 100~240V AC 50~60Hz.

USB Host		USB type-A host port.
USB Device Port		USB type-B device port is used to connect the function generator to a PC for remote control.
Counter Input		Frequency counter input.
MOD Input		Modulation input terminal.

Display

Parameter Windows	The Parameter display and edit window.
Status Tabs	Displays the current channel and setting status.
Waveform Display	Used to display the waveform
Soft Menu Keys	The function keys (F1~F5) beside the Soft Menu keys correspond to the soft keys.

Setting Up the function Generator

Background

This section describes how to adjust the handle and power up the function generator.

Adjusting the Handle

Pull out the handle sideways and rotate it.

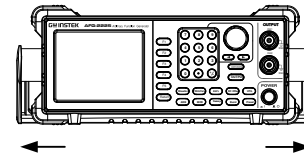

Place the AFG-2225 horizontally,



Or tilt the stand.



Place the handle vertically to hand carry.



Power Up

1. Connect the power cord to the socket on the rear panel.



2. Turn on the power switch on the front panel.

3. When the power switch is turned on the screen displays the loading screen.

The function generator is now ready to be used.

QUICK REFERENCE

This chapter describes the operation shortcuts, built-in help and factory default settings. This chapter is to be used as a quick reference, for detailed explanations on parameters, settings and limitations, please see the operation chapters.

How to use the Digital Inputs 23
How to use the Help Menu 25
Selecting a Waveform 27
- Square Wave 27
- Ramp Wave 27
- Sine Wave 28

Modulation 29
- AM 29
- FM 30
- FSK Modulation 31
- PM Modulation 32
- SUM Modulation 33

Sweep 34
Burst 35
ARB 37
- ARB–Add Built-In Waveform 37
- ARB- Add Point 37
- ARB- Add Line 38
- ARB– Output Section 38

Utility Menu 40
- Save 40
- Recall 40

Frequency Counter 41
- Frequency Counter 41

Coupling 42
- Frequency Coupling 42
- Amplitude Coupling 42

Tracking 43
Menu Tree 44
Waveform 44
ARB-Display 45
ARB-Edit 46
ARB- Built In 46
ARB-Save 47
ARB-Load 47
ARB-Output 48
MOD 48
SWEEP 49
SWEEP- More 49
Burst- N Cycle 50
Burst – Gate 50
UTIL 51
CH1/CH2 51

How to use the Digital Inputs

Background

The AFG-2225 has three main types of digital inputs: the number pad, arrow keys and scroll wheel. The following instructions will show you how to use the digital inputs to edit parameters.

1. To select a menu item, press the corresponding function keys below (F1~F5). For example the function key F1 corresponds to the Soft key "Sine".

2. To edit a digital value, use the arrow keys to move the cursor to the digit that needs to be edited.

3. Use the scroll wheel to edit the parameter. Clockwise increases the value, counter clockwise decreases the value.



4. Alternatively, the number pad can be used to set the value of a highlighted parameter.



How to use the Help Menu

Background

Every key and function has a detailed description in the help menu.

1. Press UTIL

2. Press System (F3)

3. Press Help (F2)

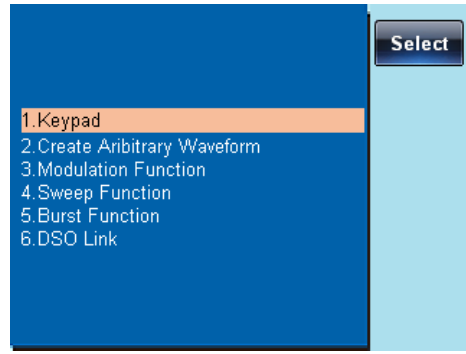

4. Use the scroll wheel to navigate to a help item. Press Select to choose the item.



Keypad	Provides help on any front panel key that is pressed.
Create Arbitrary Waveform	Provides help on creating arbitrary waveforms.
Modulation Function	Explains how to create Modulated waveforms.
Sweep Function	Provides help on the Sweep function.

Burst Function	Provides help on the Burst function.
DSO Link	Provides help on DSO link.

5. For example, select item 4 to see help on the sweep functions.

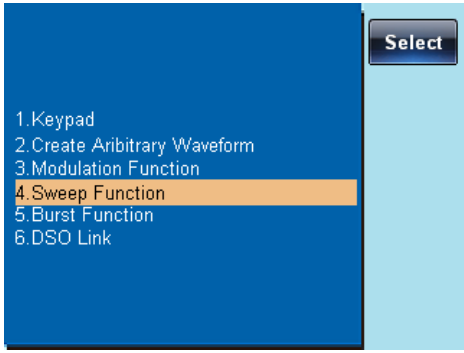

6. Use the scroll wheel to navigate the help information.

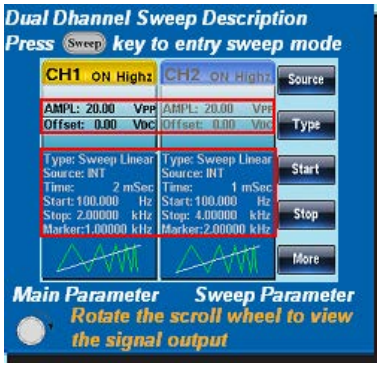

7. Press Return to return to the previous menu.

Selecting a Waveform

Square Wave

Example: Square wave, 3Vpp, 75% duty cycle, 1kHz.

Output:



1. Press Waveform and select Square (F2).

2. Press Duty (F1), 7 + 5 + %(F2).

Input: N/A

3. Press Freq/Rate, 1 + kHz (F4).

4. Press AMPL followed by, 3 + VPP (F5).

5. Press the Output key.

Ramp Wave

Example: Ramp Wave, 5Vpp, 10kHz, 50% Symmetry.

Output:



1. Press the Waveform key, and select Ramp (F4).

2. Press SYM(F1), 5 + 0 +%(F2).

Input: N/A

3. Press the Freq/Rate key then 1 + 0 + kHz (F4).

4. Press the AMPL key then 5 +VPP (F5).

5. Press the Output key.

Sine Wave

Example: Sine Wave, 10Vpp,100kHz

Output:



Input: N/A

1. Press the Waveform key and select Sine (F1).

2. Press the Freq/Rate key, followed by 1 + 0 +0 + kHz (F4).

3. Press the AMPL key, followed by 1 + 0 +VPP (F5).



4. Press the output key.

Modulation

AM

Example: AM modulation. 100Hz modulating square wave. 1kHz Sine wave carrier. 80% modulation depth.

Output:



Input: N/A

1. Press the MOD key and select AM (F1).

2. Press Waveform and select Sine (F1).

3. Press the Freq/Rate key, followed by 1 + kHz (F4).

4. Press the MOD key, select AM (F1), Shape (F4), Square (F2).

5. Press the MOD key, select AM (F1), AM Freq (F3).

6. Press 1 + 0 + 0 + Hz (F2).

7. Press the MOD key, select AM (F1), Depth (F2).

8. Press 8 + 0 + % (F1).

9. Press MOD, AM (F1), Source (F1), INT (F1).

10. Press the output key.

FM

Example: FM modulation. 100Hz modulating square wave. 1kHz Sine wave carrier. 100 Hz frequency deviation. Internal Source.

Output:



Input: N/A

1. Press the MOD key and select FM (F2).

2. Press Waveform and select Sine (F1).

3. Press the Freq/Rate key, followed by 1 + kHz (F4).

4. Press the MOD key, select FM (F2), Shape (F4), Square (F2).

5. Press the MOD key, select FM (F2), FM Freq (F3).

6. Press 1 + 0 + 0 + Hz (F2).

7. Press the MOD key, select FM (F2), Freq Dev (F2).

8. Press 1 + 0 + 0 + Hz (F3).

9. Press MOD, FM (F2), Source (F1), INT (F1).



10. Press the Output key.

FSK Modulation

Example: FSK modulation. 100Hz Hop frequency. 1kHz Carrier wave. Sine wave. 10 Hz Rate. Internal Source.

Output:



Input: N/A

1. Press the MOD key and select FSK (F3).

2. Press Waveform and select Sine (F1).

3. Press the Freq/Rate key, followed by 1 + kHz (F4).

4. Press the MOD key, select FSK (F3), FSK Rate (F3).

5. Press 1 + 0 + Hz (F2).

6. Press the MOD key, select FSK (F3), Hop Freq (F2).

7. Press 1 + 0 + 0 + Hz (F3).

8. Press MOD, FSK (F3), Source (F1), INT (F1).

9. Press the output key.

PM Modulation

Example: PM modulation. 800Hz sinusoidal carrier wave. 15 kHz modulating sine wave. 50˚ phase deviation. Internal Source.

Output:



Input: N/A

1. Press Waveform and select Sine (F1).

2. Press the MOD key and select PM (F4).

3. Press the Freq/Rate key, followed by 8 + 0 + 0 + Hz (F3).

4. Press the MOD key, select PM (F4), Shape (F4), Sine (F1).

5. Press MOD, then PM (F4), PM Freq (F3).

6. Press 1 + 5 + kHz (F3).

7. Press MOD, PM (F4), PM Dev (F2).

8. Press 5 + 0 + Degree (F1).

9. Press MOD, PM (F4), Source (F1), INT (F1).

10. Press the Output key.

SUM Modulation

Example: SUM modulation. 100Hz modulating square wave, 1kHz sinusoidal carrier wave, 50% SUM amplitude, internal source.

Output:



Input: N/A

1. Press the MOD key, then SUM (F5).

2. Press Waveform, and select Sine (F1).

3. Press Freq/Rate followed by 1 + kHz (F4). 

4. Press the MOD key, SUM (F5), Shape (F4), Square (F2).

5. Press the MOD key and select SUM (F5), SUM Freq (F3).

6. Press 1 + 0 + 0 + Hz (F2). 

7. Press the MOD key and select SUM (F5), SUM Ampl (F2).

8. Press 5 + 0 + % (F1).

9. Press MOD, SUM (F5), Source (F1), INT (F1).



10. Press the Output key.

Sweep

Example: Frequency Sweep. Start Frequency 10mHz, Stop frequency 1MHz. Log sweep, 1 second sweep, Marker Frequency 550 Hz, Manual Trigger.

Output:



1. Press Sweep, Start (F3).

2. Press 1 + 0 + mHz (F2).

3. Press Sweep, Stop (F4).

Input: N/A

4. Press 1 + MHz (F5).

5. Press Sweep, Type (F2), Log (F2).

6. Press Sweep, More (F5), SWP Time (F1).

7. Press 1 + SEC (F2).

8. Press Sweep, More (F5), Marker (F4), ON/OFF (F2), Freq (F1).

9. Press 5 + 5 + 0 + Hz (F3).



10. Press the Output key.

11. Press Sweep, Source (F1), Manual (F3), Trigger (F1).

Burst

Example: Burst Mode, N-Cycle (Internally triggered), 1kHz burst frequency, Burst count = 5, 10 ms Burst period, 0˚ burst phase, Internal trigger, 10 us delay, rising edge trigger out

Output:



Input: N/A

1. Press FREQ/Rate 1 kHz (F4).



2. Press Burst, N Cycle (F1), Cycles (F1).

3. Press 5 + Cyc (F2).

4. Press Burst, N Cycle (F1), Period (F4).

5. Press 1 +0 + msec (F2).

6. Press Burst, N Cycle (F1), Phase (F3).

7. Press 0 + Degree (F2).

8. Press Burst, N Cycle (F1), TRIG set (F5), INT (F1).



9. Press Burst, N Cycle (F1), TRIG set (F5), Delay (F4).

10. Press 1 + 0 + uSEC (F2).

11. Press Burst, N Cycle (F1), TRIG set (F5), TRIG out (F5), ON/OFF (F3), Rise (F1).

12. Press the Output key.

ARB

ARB–Add Built-In Waveform

Example: ARB Mode, Exponential Rise. Start 0, Length 100, Scale 327.

Output:



1. Press ARB, Built in (F3), Wave (F4), Math(F2), use the scroll wheel to select Exporise and then press Select(F5).



2. Press Start (F1), 0 + Enter (F2), Return.

3. Press Length (F2), 100, Enter (F2), Return.

4. Press Scale (F3), 327, Enter (F2), Return, Done (F5).

ARB- Add Point

Example: ARB Mode, Add point, Address 40, data 300.

Output:



1. Press ARB, Edit (F2), Point (F1), Address (F1)

2. Press 4 + 0 + Enter (F2), Return

3. Press Data (F2), 3+0+0, Enter (F2).

ARB- Add Line

Example: ARB Mode, Add line, Address:Data (10:30, 50:100)

Output:



1. Press ARB, Edit (F2), Line (F2), Start ADD (F1).

2. Press 1 + 0 + Enter (F2), Return.

3. Press Start Data (F2), 3 + 0, Enter (F2), Return.



4. Press Stop ADD (F3), 5 + 0, Enter (F2), Return.



5. Press Stop Data (F4), 1 + 0 + 0, Enter (F2), Return, Done (F5).



ARB– Output Section

Example: ARB Mode, Output ARB Waveform, Start 0, Length 1000.

Output:



1. Press ARB, Output (F4).

2. Press Start (F1), 0 + Enter (F2), Return.



3. Press Length (F2), 1 + 0 + 0, Enter (F2), Return.

Utility Menu

Save

Example: Save to Memory file #5.

1. Press UTIL, Memory (F1), Store (F1).

2. Choose a setting using the scroll wheel and press Done (F5).

Recall

Example: Recall Memory file #5.

1. Press UTIL, Memory (F1), Recall (F2).

2. Choose a setting using the scroll wheel and press Done (F5).

Frequency Counter

Frequency Counter

Example: Turn on the frequency counter. Gate time: 1 second.

Output: N/A

Input:



1. Press UTIL, Counter (F5).

2. Press Gate Time (F1), and press 1 Sec (F3) to choose a gate time of 1 second.

3. Connect the signal of interest to the Frequency counter input on the rear panel.

Coupling

Frequency Coupling

Example: Frequency Coupling

1. Press UTIL, Dual Chan (F4) to enter the coupling function.

2. Press Freq Cpl (F1) to select the frequency coupling function.

3. Press Offset (F2). The offset is the frequency difference between CH1 and CH2. Use the number keys or scroll wheel to enter the offset.

Amplitude Coupling

Example: Amplitude Coupling

1. Press UTIL, Dual Chan (F4) to enter the coupling function.

2. Press Ampl Cpl (F2), ON (F1) to select the amplitude coupling function.

3. Couples the amplitude and offset between both channels. Any changes in amplitude in the current channel are reflected in the other channel.

Tracking

Example: Tracking

1. Press UTIL, Dual Chan (F4) to enter the coupling function.

2. Press Tracking (F3), ON (F2) to turn on the tracking function.

3. When tracking is turned on, parameters such as amplitude and frequency from the current channel are mirrored on the other channel.

Menu Tree

Conventions

Use the menu trees as a handy reference for the function generator functions and properties. The AFG-2225 menu system is arranged in a hierarchical tree. Each hierarchical level can be navigated with the operation or soft menu keys. Pressing the Return key will return you to the previous menu level.

Waveform

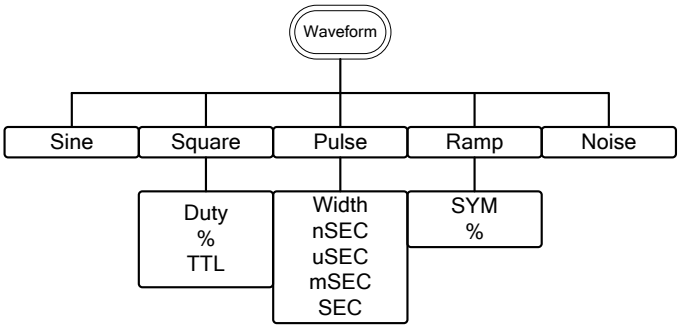

ARB-Display

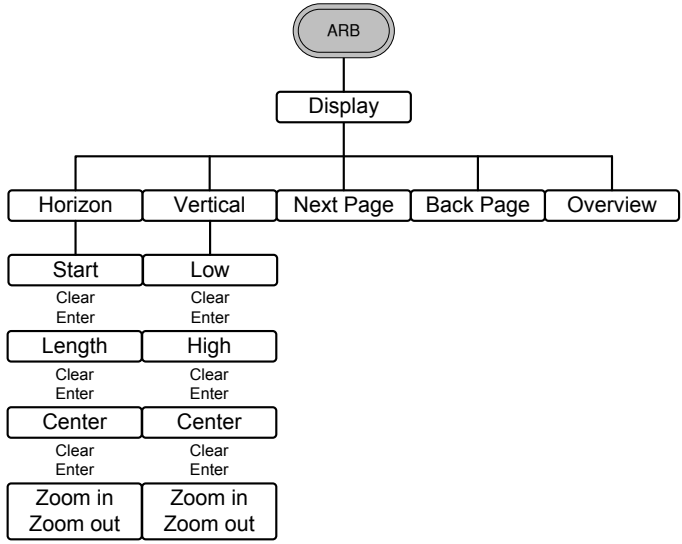
ARB
Display
Horizon
Vertical
Next Page
Back Page
Overview
Start
Clear
Enter
Length
Clear
Enter
Center
Clear
Enter
Zoom in
Zoom out
Low
Clear
Enter
High
Clear
Enter
Center
Clear
Enter
Zoom in
Zoom out

ARB-Edit

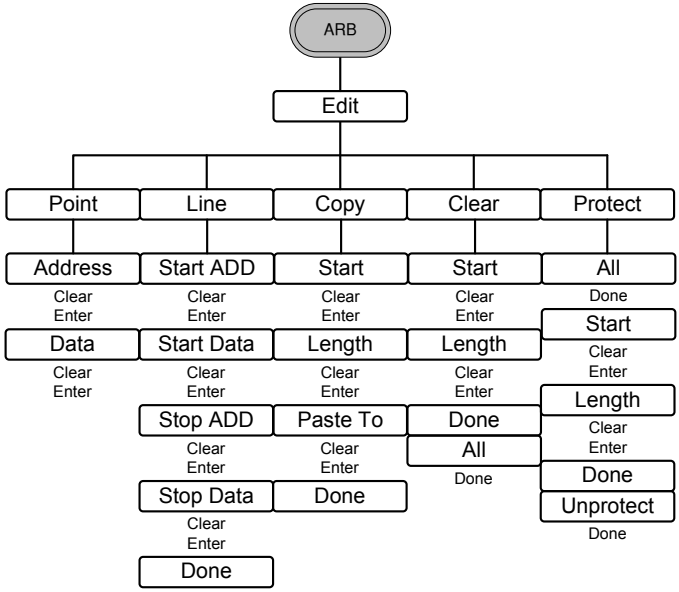

ARB- Built In

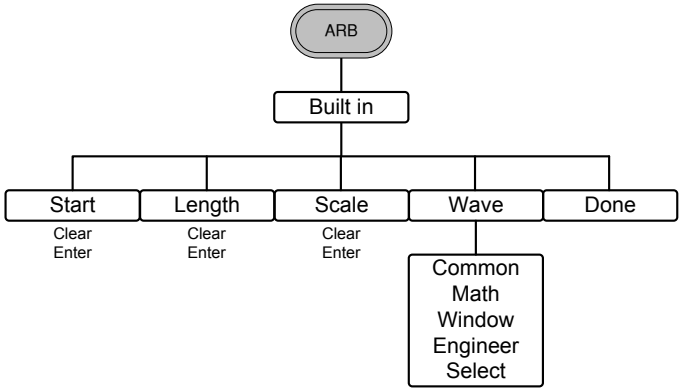

ARB-Save

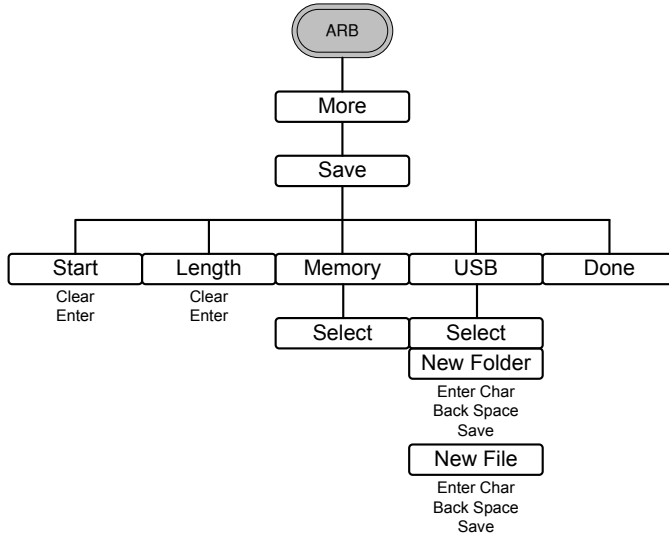

ARB-Load

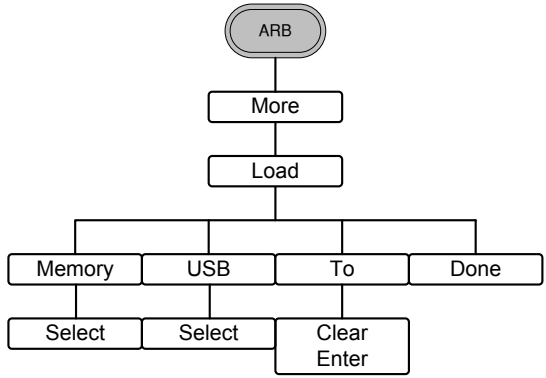

ARB-Output

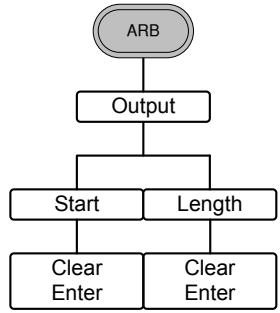

MOD

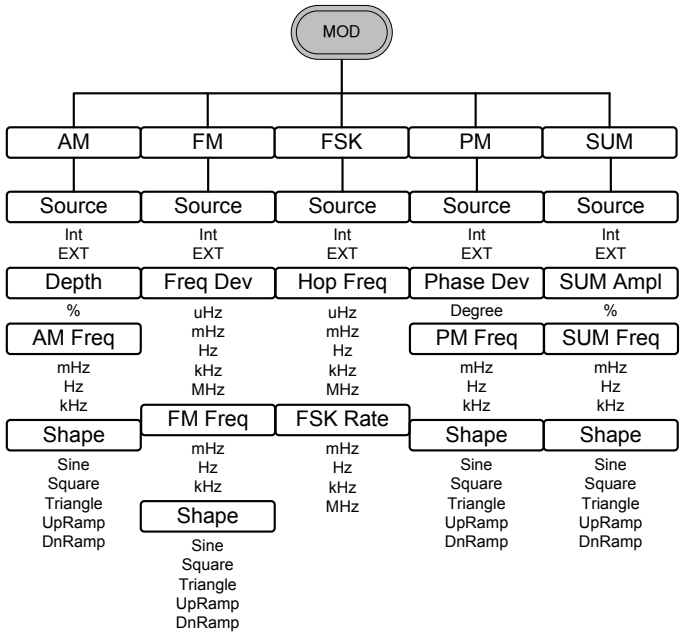

SWEEP

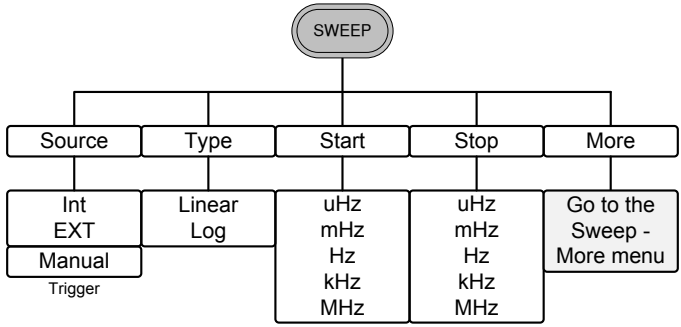

SWEEP- More

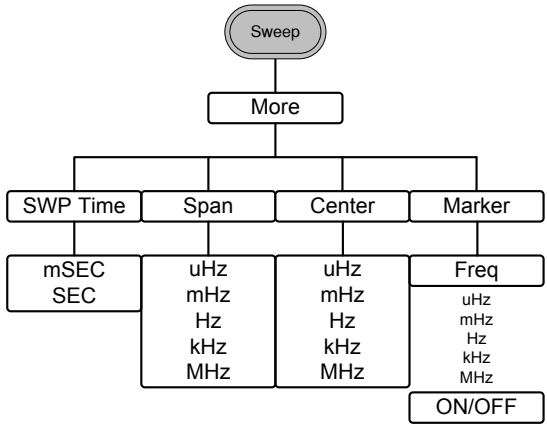

Burst- N Cycle

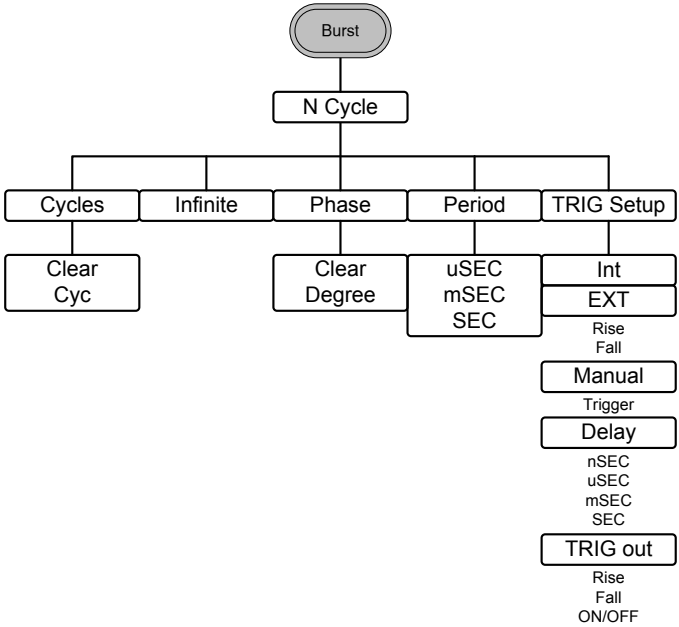

Burst – Gate

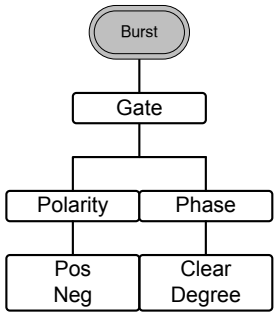

UTIL

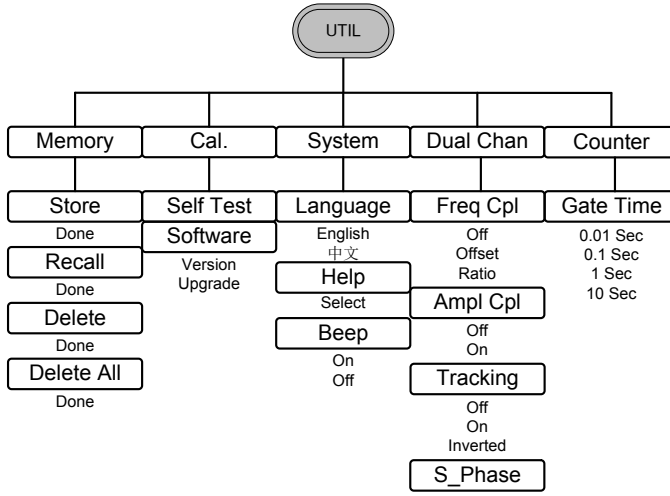
UTIL
Memory
Cal.
System
Dual Chan
Counter
Store
Done
Recall
Done
Delete
Done
Delete All
Done
Self Test
Software
Version
Upgrade
Language
English
中文
Help
Select
Beep
On
Off
Freq Cpl
Off
Offset
Ratio
Ampl Cpl
Off
On
Tracking
Off
On
Inverted
S_Phase
Gate Time
0.01 Sec
0.1 Sec
1 Sec
10 Sec

CH1/CH2

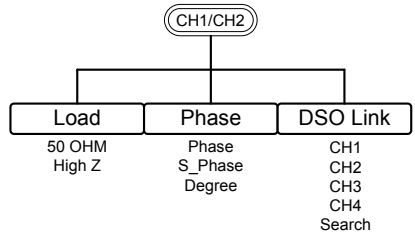
CH1/CH2
Load
50 OHM
High Z
Phase
Phase
S_Phase
Degree
DSO Link
CH1
CH2
CH3
CH4
Search

Default Settings

The Preset key is used to restore the default panel settings.

Output Settings	Function	Sine Wave
	Frequency	1kHz
	Amplitude	3.000 Vpp
	Offset	0.00V dc
	Output units	Vpp
	Output terminal	50Ω
Modulation (AM/FM/FSK/ PM/SUM)	Carrier wave	1kHz sine wave
	Modulation wave	100Hz sine wave
	AM depth	100%
	FM deviation	100Hz
	FSK hop frequency	100Hz
	FSK frequency	10Hz
	PM phase deviation	180°
	SUM amplitude	50%
	Modem status	Off
Sweep	Start/Stop frequency	100Hz/1kHz
	Sweep time	1s
	Sweep type	Linear
	Sweep status	Off

Burst	Burst frequency	1kHz
	Ncycle	1
	Burst period	10ms
	Burst starting phase	0˚
	Burst status	Off
System Settings	Power off signal	On
	Display mode	On
	Error queue	Cleared
	Memory settings	No change
	Output	Off
Trigger	Trigger source	Internal (immediate)
Calibration	Calibration Menu	Restricted

OPERATION

The Operation chapter shows how to output basic waveform functions. For details on modulation, sweep, burst and arbitrary waveforms, please see the Modulation and Arbitrary waveform chapters on pages 64 and 147.

Select a Waveform 55
Sine Wave 55
Square Wave 56
Setting the Pulse Width 57
Setting a Ramp Waveform 58
Selecting a Noise Waveform 59
Setting the Frequency 60
Setting the Amplitude 62
Setting the DC Offset 63

Select a Waveform

The AFG-2225 can output 5 standard waveforms: sine, square, pulse, ramp and noise.

Sine Wave

Panel Operation

1. Press the Waveformkey.

2. Press F1 (Sine).

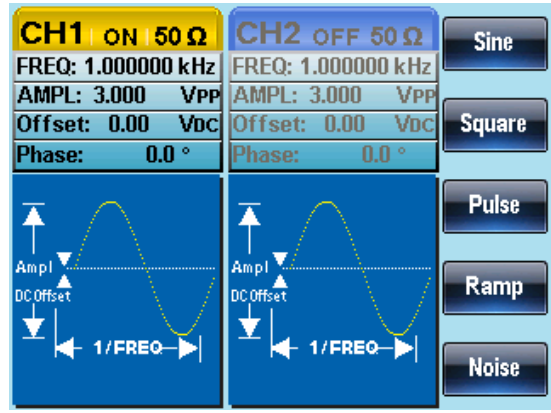

Square Wave

Panel Operation

1. Press the Waveform key.

2. Press F2 (Square) to create a square waveform.

3. Press F1 (Duty). The Duty parameter will be highlighted in the parameter window.

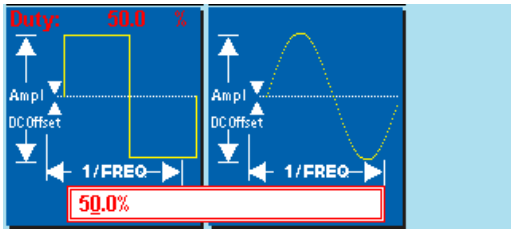

4. Use the arrow keys and scroll wheel or number pad to enter the Duty range.



5. Press F2 (%) to select % units.

Range	Frequency	Duty Range
	≤100kHz	1.0%~99.0%
	100kHz~≤1MHz	10.0%~90.0%
	>1MHz~25MHz	50% (Fixed)

TTL function is to set the amplitude of the current square wave at 2.5Vpp,and DC Offset at 1.25Vdc.

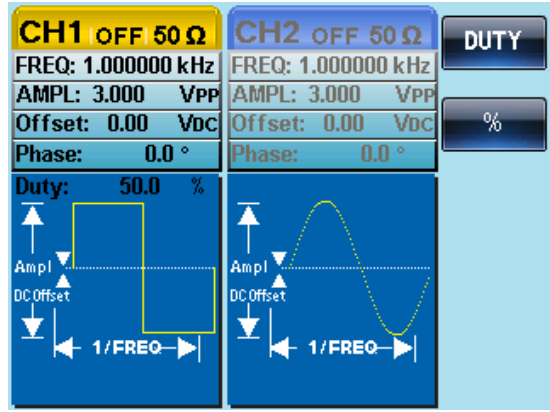

Setting the Pulse Width

Panel Operation

1. Press the Waveform key.

2. Press F3 (Pulse) to create a pulse width waveform.

3. Press F1 (Width). The Width parameter will be highlighted in the parameter window.

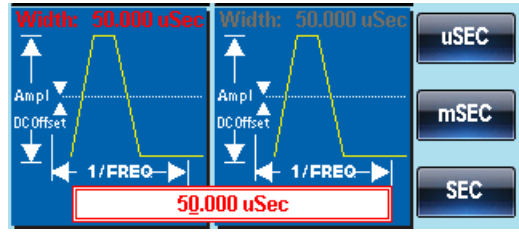

4. Use the arrow keys and scroll wheel or number pad to enter the pulse width.



5. Press F2~F5 choose the unit range.



Range	Pulse Width	20ns~1999.9s
Note	Minimum Pulse Width	Frequency ≤ 25MHz: 20ns pulse width. Frequency ≤ 100 kHZ: 1/4096 duty cycle.
	Resolution	Frequency ≤ 25MHz: 20ns pulse width. Frequency ≤100 kHZ: 1/4096 duty cycle.

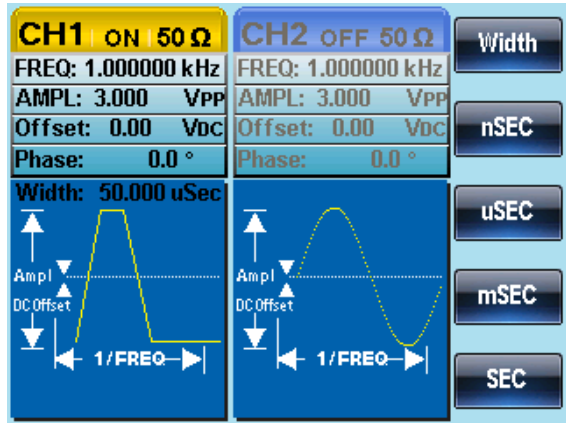

Setting a Ramp Waveform

Panel Operation

1. Press the Waveform key.

2. Press F4 (Ramp) to create a ramp waveform.

3. Press F1 (SYM). The SYM parameter will be highlighted in the parameter window.

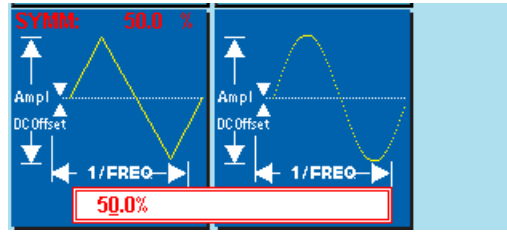

4. Use the arrow keys and scroll wheel or number pad to enter the symmetry percentage.



5. Press F2 (%) to choose % units.

Range Symmetry 0%~100%

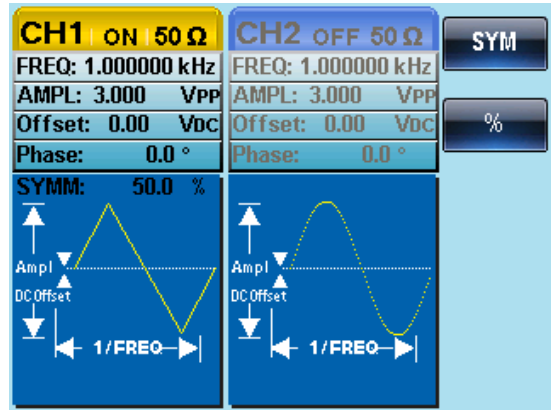

Selecting a Noise Waveform

Panel Operation

1. Press the Waveform key.

2. Press F5 (Noise).

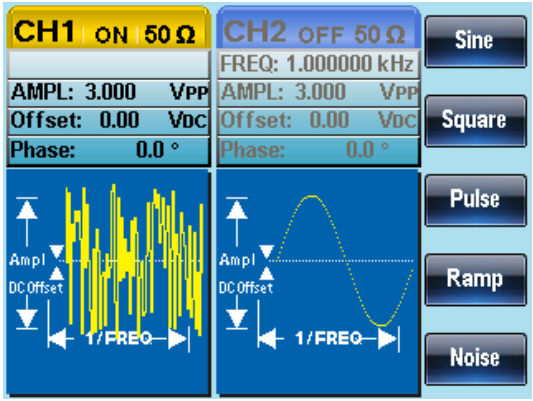

Setting the Frequency

Panel Operation

1. Press the FREQ/Rate key.

2. The FREQ parameter will become highlighted in the parameter window.

3. Use the arrow keys and scroll wheel or number pad to enter the frequency.



4. Choose a frequency unit by pressing F1~F5.



Range

Sine wave	1μHz~25MHz
Square wave	1μHz~25MHz
Pulse wave	500μHz~25MHz

Ramp wave 1μHz~1MHz

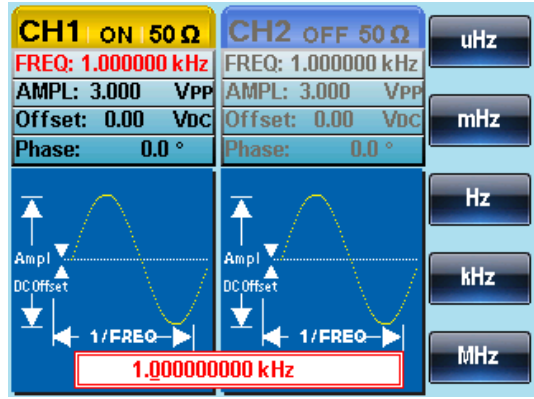

Setting the Amplitude

Panel Operation

1. Press the AMPL key.

2. The AMPL parameter will become highlighted in the parameter window.

3. Use the arrow keys and scroll wheel or number pad to enter the amplitude.



4. Choose a unit type by pressing F1~F5.



	50Ω load	High Z
Range	1mVpp~10Vpp	2mVpp~20Vpp
Unit	Vpp, Vrms, dBm	

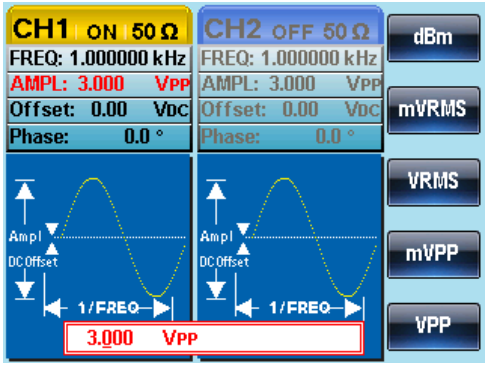

Setting the DC Offset

Panel Operation

1. Press the DC Offset key.

2. The DC Offset parameter will become highlighted in the parameter window.

3. Use the arrow keys and scroll wheel or number pad to enter the DC Offset.



4. Press F1 (mVDC) or F2 (VDC) to choose a voltage range.

	50Ω load	High Z
Range	±5Vpk	±10Vpk

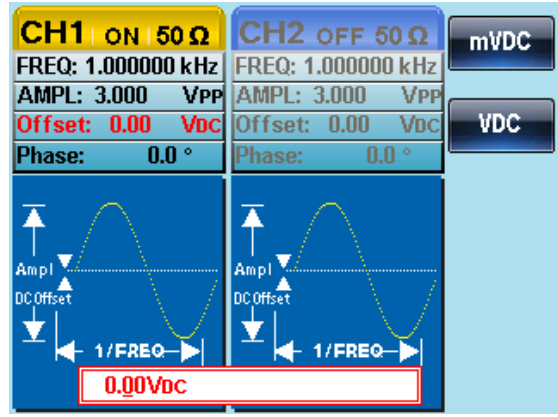

MODULATION

The AFG-2225 Series Arbitrary Function Generators are able to produce AM, FM, FSK, PM and SUM modulated waveforms. Depending on the type of waveform produced, different modulation parameters can be set. Only one modulation mode can be active at any one time. The function generator also will not allow sweep or burst mode to be used with AM/FM. Activating a modulation mode will turn the previous modulation mode off.

Amplitude Modulation (AM) 66
- Selecting AM Modulation 67
- AM Carrier Shape 67
- Carrier Frequency 68
- Modulating Wave Shape 69
- AM Frequency 70
- Modulation Depth 72
- Selecting the (AM) Modulation Source 73

Frequency Modulation (FM) 75
- Selecting Frequency Modulation (FM) 76
- FMCarrier Shape 76
- FM Carrier Frequency 77
- FM Wave Shape 78
- FM Frequency 79
- Frequency Deviation 81
- Selecting (FM) Modulation Source 82

Frequency Shift Keying (FSK) Modulation 84
- Selecting FSK Modulation 85
- FSK Carrier Shape 85
- FSK Carrier Frequency 86
- FSK Hop Frequency 87
- FSK Rate 88
- FSK Source 90

Phase Modulation (PM) 91
- Selecting Phase Modulation (PM) 92
- PM Carrier Waveform 93
- PM Carrier Frequency 93

PM Wave Shape 94
PM Frequency 95
Phase Deviation 97
Select the PM Source 98
SUM modulation 100
Selecting SUM modulation 101
SUM Carrier Waveform 101
SUM Carrier Frequency 102
SUM Waveform 103
Modulating Waveform Frequency 104
SUM Amplitude 105
Select the SUM Amplitude Source 106
Frequency Sweep 108
Selecting Sweep Mode 109
Setting Start and Stop Frequency 109
Center Frequency and Span 111
Sweep Mode 113
Sweep Time 114
Marker Frequency 115
Sweep Trigger Source 116
Burst Mode 118
Selecting Burst Mode 119
Burst Modes 119
Burst Frequency 120
Burst Cycle/Burst Count 121
Infinite Burst Count 123
Burst Period 123
Burst Phase 125
Burst Trigger Source 126
Burst Delay 128
Burst Trigger Output 129

Amplitude Modulation (AM)

An AM waveform is produced from a carrier waveform and a modulating waveform. The amplitude of the modulated carrier waveform depends on the amplitude of the modulating waveform. The AFG-2225 function generator can set the carrier frequency, amplitude and offset as well as internal or external modulation sources.

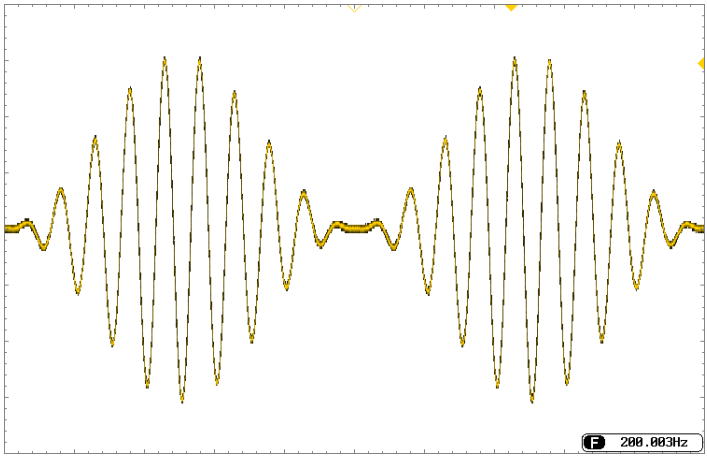

Selecting AM Modulation

Panel Operation

1. Press the MOD key.

2. Press F1 (AM).

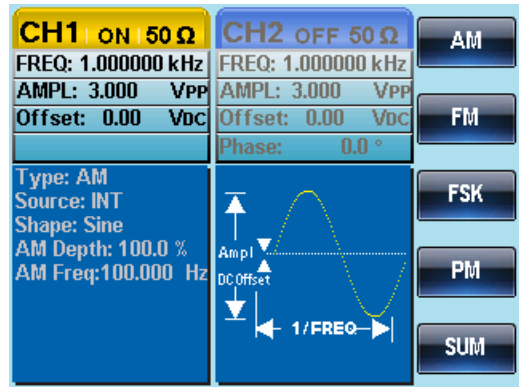

AM Carrier Shape

Background

Sine, square, ramp, pulse or arbitrary waveforms can be used as the carrier shape. The default waveform shape is set to sine. Noise is not available as a carrier shape. Before the carrier shape can be selected, choose AM modulation mode, see above.

Select a Standard Carrier Shape

1. Press the Waveform key.

2. Press F1~F4 to choose the carrier wave shape.



Select an Arbitrary Waveform Carrier Shape.	3. See the Arbitrary waveform quick reference or chapter to use an arbitrary waveform.	Page 37 Page 147

Range	AM Carrier Shape	sine, square, Ramp,Pulse, arbitrary waveform

Carrier Frequency

The maximum carrier frequency depends on the carrier shape selected. The default carrier frequency for all carrier shapes is 1kHz.

Panel Operation

1. With a carrier waveform selected, press the FREQ/Rate key.

2. The FREQ parameter will become highlighted in the parameter window.

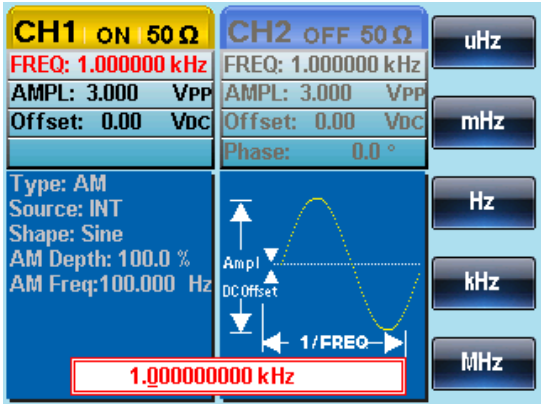

3. Use the arrow keys and scroll wheel or number pad to enter the carrier frequency.



4. Press F1~F5 to select the frequency range.



Range	Carrier Shape	Carrier Frequency
	Sine wave	1μHz~ 25MHz
	Square wave	1μHz~25MHz
	Ramp wave	1μHz~1MHz
	Pulse wave	500uHz~25MHz
	Default frequency	1 kHz

Modulating Wave Shape

The function generator can accept internal as well as external sources. The AFG-2225 has sine, square, triangle, up ramp and down ramp modulating waveform shapes. Sine waves are the default wave shape.

Panel Operation

1. Press the MOD key.

2. Press F1 (AM).

3. Press F4 (Shape).

4. Press F1 ~ F5 to select the waveform shape.



5. Press Return to return to the previous menu.



Note		
	Square wave	50% Duty cycle
	UpRamp	100% Symmetry
	Triangle	50% Symmetry
	DnRamp	0% Symmetry

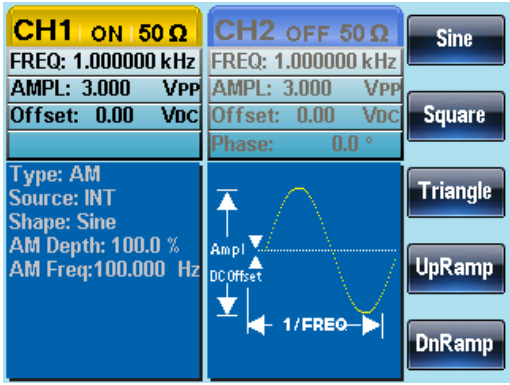

AM Frequency

The frequency of the modulation waveform (AM Frequency) can be set from 2mHz to 20kHz.

Panel Operation

1. Press the MOD key.

2. Press F1 (AM).

3. Press F3 (AM Freq)

4. The AM Freq parameter will become highlighted in the Waveform display area.

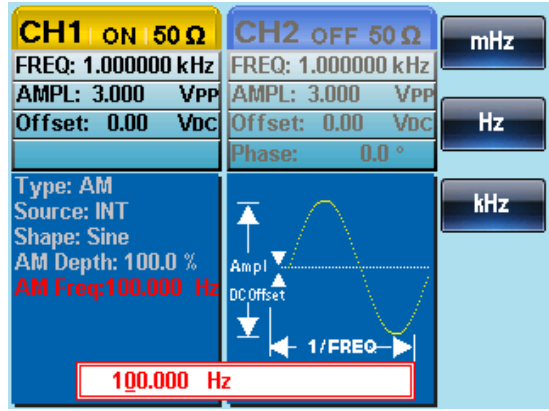

5. Use the arrow keys and scroll wheel or number pad to enter the AM frequency.



6. Press F1~F3 to select the frequency range.



Range	Modulation frequency	2mHz~20kHz
	Default frequency	100Hz

Modulation Depth

Modulation depth is the ratio (as a percentage) of the unmodulated carrier amplitude and the minimum amplitude deviation of the modulated waveform. In other words, modulation depth is the maximum amplitude of the modulated waveform compared to the carrier waveform as a percentage.

Panel Operation

1. Press the MOD key.

2. Press F1 (AM).

3. Press F2 (Depth).

4. The AM Depth parameter will become highlighted in the waveform display area.

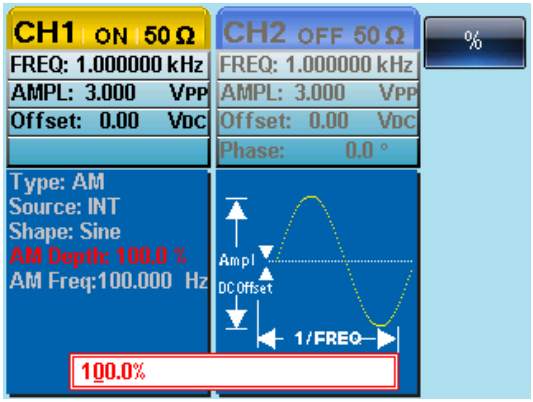

5. Use the arrow keys and scroll wheel or number pad to enter the AM depth.



6. Press F1 (%) to choose % units.

Range	Depth	0%~120%
	Default depth	100%

Note

When the modulation depth is greater than 100%, the output cannot exceed ±5VPeak (10kΩ load).

If an external modulation source is selected, modulation depth is limited to ± 5V from the MOD INPUT terminal on the rear panel. For example, if the modulation depth is set to 100%, then the maximum amplitude is +5V, and the minimum amplitude is -5V.

Selecting the (AM) Modulation Source

The function generator will accept an internal or external source for AM modulation. The default source is internal.

Panel Operation

1. Press the MOD key.

2. Press F1 (AM).

3. Press F1 (Source).

4. Press F1 (INT) or F2 (EXT) to select the modulation source.



5. Press Return to go back to the previous menu.

External Source

Use the MOD INPUT terminal on the rear panel when using an external source.



Note

If an external modulation source is selected, modulation depth is limited to ± 5V from the MOD INPUT terminal on the rear panel. For example, if modulation depth is set to 100%, then the maximum amplitude is +5V, and the minimum amplitude is -5V.

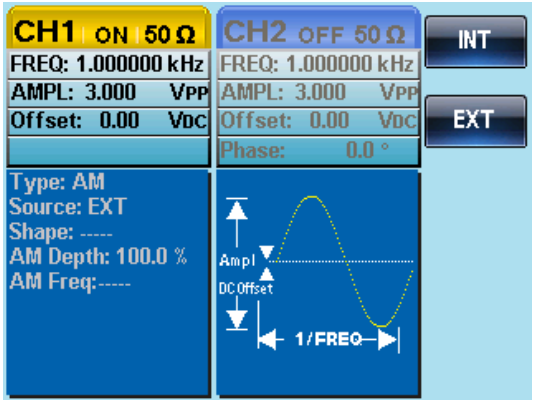

Frequency Modulation (FM)

A FM waveform is produced from a carrier waveform and a modulating waveform. The instantaneous frequency of the carrier waveform varies with the magnitude of the modulating waveform. When using the AFG-2225 function generator, only one type of modulated waveform can be created at any one time.

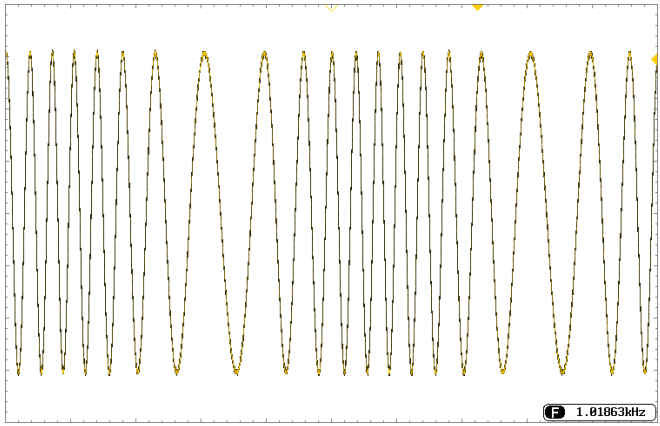

Selecting Frequency Modulation (FM)

When FM is selected, the modulated waveform depends on the carrier frequency, the output amplitude and offset voltage.

Panel Operation

1. Press the MOD key.

2. Press F2 (FM).

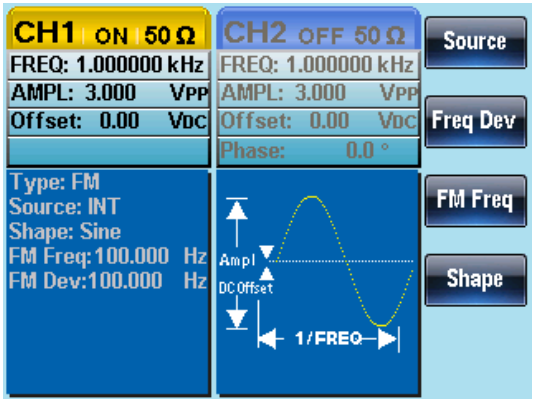

FMCarrier Shape

Background

The default waveform shape is set to sine. Noise and pulse waveforms cannot be used as a carrier wave.

Panel Operation

1. Press the Waveform key.

2. Press F1~F4 to select the carrier shape.



Range	Carrier Shape	Sine, Square, Ramp.

FM Carrier Frequency

When using the AFG-2225 function generator, the carrier frequency must be equal to or greater than the frequency deviation. If the frequency deviation is set to value greater than the carrier frequency, the deviation is set to the maximum allowed. The maximum frequency of the carrier wave depends on the waveform shape chosen.

Panel Operation

1. To select the carrier frequency, press the FREQ/Rate key.

2. The FREQ parameter will become highlighted in the parameter window.

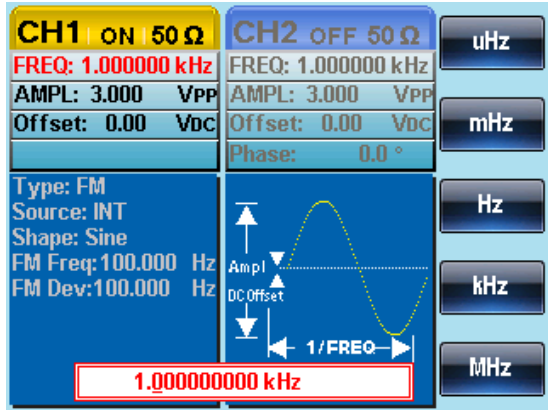

3. Use the arrow keys and scroll wheel or number pad to enter the carrier frequency.



4. Press F1~F5 to select the frequency unit.



Range	Carrier Shape	Carrier Frequency

	Sine	1μHz~25MH
	Square	1μHz~15MHz
	Ramp	1μHz~1MHz
	Default frequency	1kHz

FM Wave Shape

The function generator can accept internal as well as external sources. The AFG-2225 has sine, square, triangle, positive and negative ramps (UpRamp, DnRamp) as the internal modulating waveform shapes. Sine is the default wave shape.

Background

1. Select MOD.

2. Press F2 (FM).

3. Press F4 (Shape).

4. Press F1 ~ F5 to select the waveform shape.



5. Press Return to return to the previous menu.

Range	Square wave	50% Duty cycle
	UpRamp	100% Symmetry
	Triangle	50% Symmetry
	DnRamp	0% Symmetry

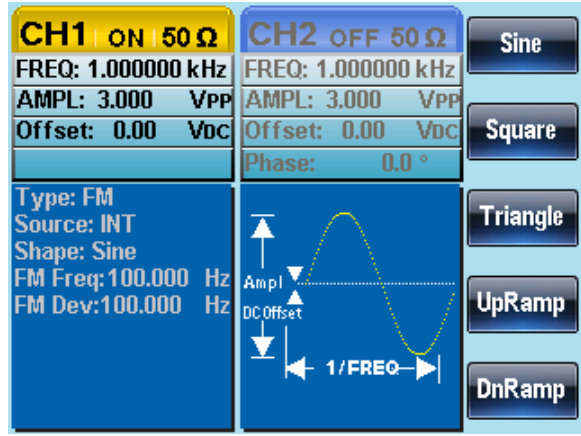

FM Frequency

The frequency of the modulation waveform (FM Frequency) can be set from 2mHz to 20kHz.

Panel Operation

1. Press the MOD key.

2. Press F2 (FM).

3. Press F3 (FM Freq).

4. The FM Freq parameter will become highlighted in waveform display panel.

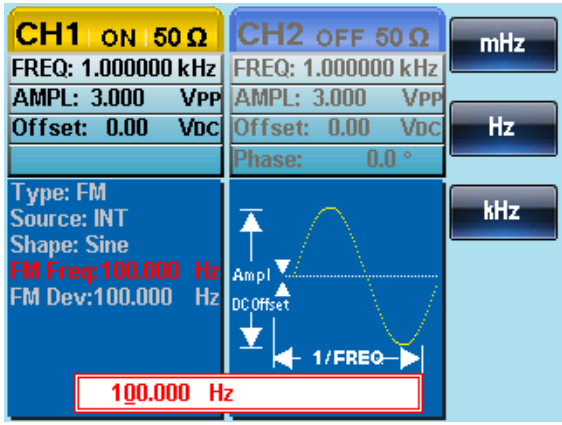

5. Use the arrow keys and scroll wheel or number pad to enter the FM frequency.



6. Press F1~F3 to select the frequency unit.



Range	Modulation frequency	2mHz~20kHz
	Default frequency	100Hz

Frequency Deviation

The frequency deviation is the peak frequency deviation from the carrier wave and the modulated wave.

Panel Operation

1. Press the MOD key.

2. Press F2 (FM).

3. Press F2 (Freq Dev).

4. The Freq Dev parameter will become highlighted in the waveform display panel.

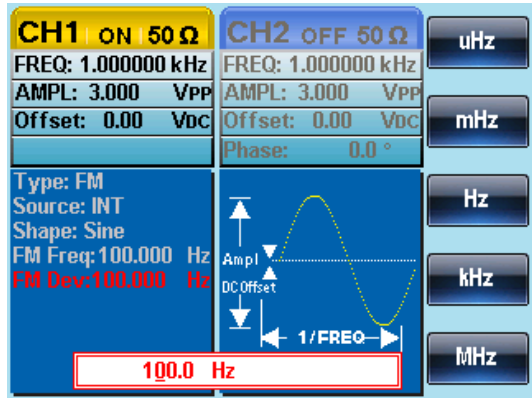

5. Use the arrow keys and scroll wheel or number pad to enter the frequency deviation.



6. Press F1~ F5 to choose the frequency units.



Range	Frequency Deviation	DC~25MHz DC~15MHz(square) DC~1MHz (Ramp)
	Default depth	100Hz

Selecting (FM) Modulation Source

The function generator will accept an internal or external source for FM modulation. The default source is internal.

Panel Operation

1. Press the MOD key.

2. Press F2 (FM).

3. Press F1 (Source).

4. To select the source, press F1 (Internal) or F2 (External).



5. Press Return to return to the previous menu.

External Source

Use the MOD INPUT terminal on the rear panel when using an external source.



Note

If an external modulating source is selected, the frequency deviation is limited to the ± 5V MOD INPUT terminal on the rear panel. The frequency deviation is proportional to the signal level of the modulation in voltage. For example, if the modulation in voltage is +5V, then the frequency deviation would be equal to the set frequency deviation. Lower signal levels reduce the frequency deviation while negative voltage levels produce frequency deviations with frequencies below the carrier waveform.

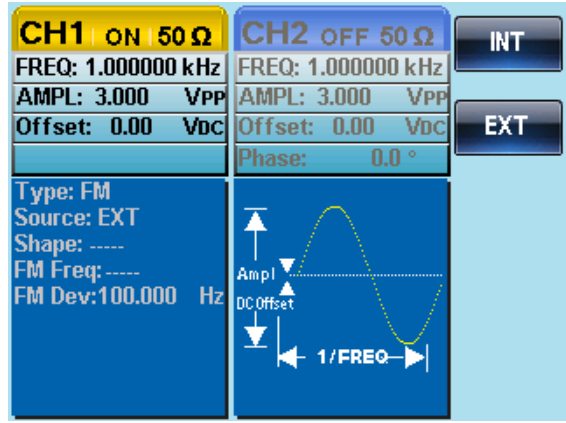

Frequency Shift Keying (FSK) Modulation

Frequency Shift Keying Modulation is used to shift the frequency output of the function generator between two preset frequencies (carrier frequency, hop frequency). The frequency at which the carrier and hop frequency shift is determined by the internal rate generator or the voltage level from the Trigger INPUT terminal on the rear panel.

Only one modulation mode can be used at once. When FSK modulation is enabled, any other modulation modes will be disabled. Sweep and Burst also cannot be used with FSK modulation. Enabling FSK will disable Sweep or Burst mode.

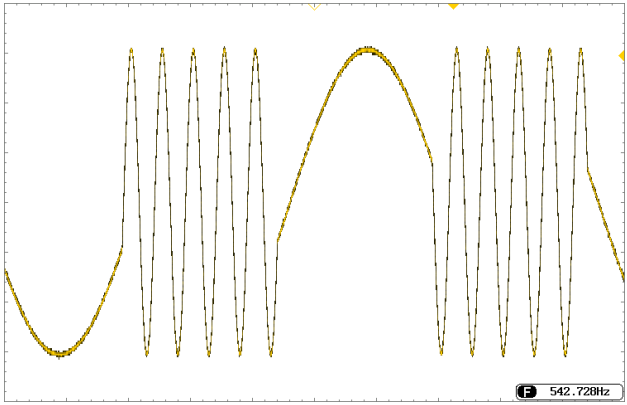

Selecting FSK Modulation

When using FSK mode, the output waveform uses the default settings for carrier frequency, amplitude and offset voltage.

Panel Operation

1. Press the MOD key.

2. Press F3 (FSK).

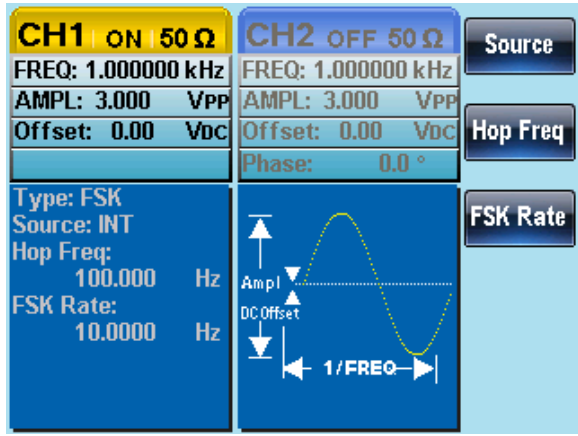

FSK Carrier Shape

Background

The default waveform shape is set to sine. Noise waveforms cannot be used as carrier waves.

Panel Operation

1. Press the Waveform key.

2. Press F1~F4 to choose the carrier wave shape.



Range	Carrier Shape	Sine, Square, Pulse, Ramp

FSK Carrier Frequency

The maximum carrier frequency depends on the carrier shape. The default carrier frequency for all carrier shapes is 1kHz. The voltage level of the Trigger INPUT signal controls the output frequency when EXT is selected. When the Trigger INPUT signal is logically low the carrier frequency is output and when the signal is logically high, the hop frequency is output.

Panel Operation

1. Press the FREQ/Rate key to select the carrier frequency.

2. The FREQ parameter will become highlighted in the parameter window.

3. Use the arrow keys and scroll wheel or number pad to enter the carrier frequency.



4. Press F1~F5 to select the FSK frequency units.



Range	Carrier Shape	Carrier Frequency
	Sine wave	1μHz~25MHz
	Square wave	1μHz~15MHz
	Ramp wave	1μHz~1MHz
	Pulse wave	500μHz~15MHz
	Default frequency	1kHz

FSK Hop Frequency

The default Hop frequency for all waveform shapes is 100 Hz. A square wave with a duty cycle of 50% is used for the internal modulation waveform. The voltage level of the Trigger INPUT signal controls the output frequency when EXT is selected. When the Trigger INPUT signal is logically low the carrier frequency is output and when the signal is logically high, the hop frequency is output.

Panel Operation

1. Press the MOD key.

2. Press F3 (FSK).

3. Press F2 (Hop Freq).

4. The Hop Freq parameter will become highlighted in the Waveform Display area.

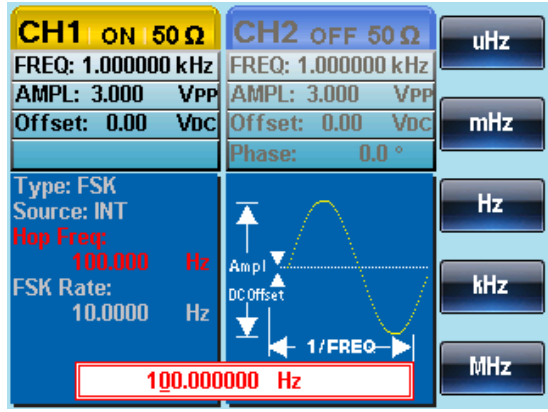

5. Use the arrow keys and scroll wheel or number pad to enter the hop frequency.



6. Press F1~F5 to select the frequency range.



Range	Waveform	Carrier Frequency
	Sine wave	1μHz~25MHz
	Square wave	1μHz~15MHz
	Ramp wave	1μHz~1MHz
	Pulse wave	500μHz~15MHz
	Default frequency	100Hz

FSK Rate

FSK Rate function is used to determine rate at which the output frequency changes between the carrier and hop frequencies. The FSK Rate function only applies to internal FSK sources.

Panel Operation

1. Select the MOD key.

2. Press F3 (FSK).

3. Press F3 (FSK Rate).

4. The FSK Rate parameter will become highlighted in the waveform display area.

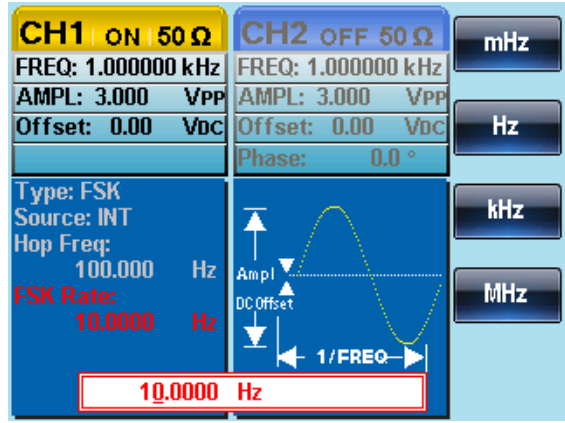

5. The arrow keys and scroll wheel or number pad to enter the FSK rate.



6. Press F1~F4 to select the frequency unit.



Range	FSK Rate	2mHz~100kHz
	Default	10Hz
Note	If an external source is selected, FSK Rate settings are ignored.	

FSK Source

The AFG-2225 accepts internal and external FSK sources, with internal as the default source. When the FSK source is set to internal, the FSK rate is configured using the FSK Rate function. When an external source is selected the FSK rate is equal to the frequency of the Trigger INPUT signal on the rear panel.

Panel Operation

1. Press the MOD key.

2. Press F3 (FSK).

3. Press F1 (Source).

4. Press F1 (Internal) or F2 (External) to select the FSK source.



5. Press Return to return to the previous menu.

Note

Note that the Trigger INPUT terminal cannot configure edge polarity.

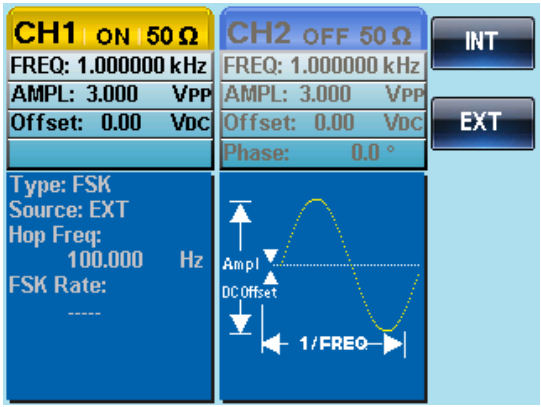

Phase Modulation (PM)

The phase deviation of the carrier waveform deviates from a reference phase value in proportion to changes in the modulating waveform.

Only one mode of modulation can be enabled at any one time. If PM is enabled, any other modulation mode will be disabled. Likewise, burst and sweep modes cannot be used with PM and will be disabled when PM is enabled.

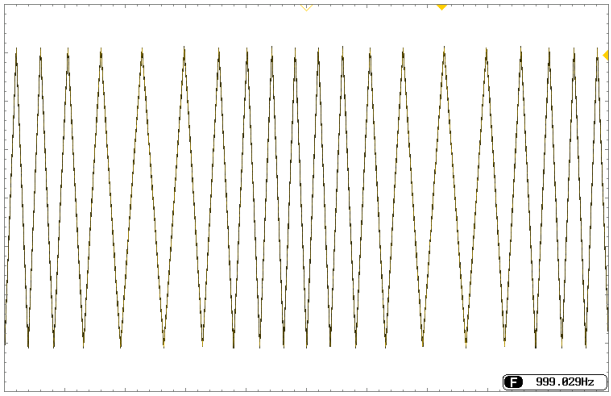

Selecting Phase Modulation (PM)

When selecting PM, the current setting of the carrier frequency, the amplitude modulation frequency, output, and offset voltage must be considered.

Panel Operation

1. Press the MOD key.

2. Press F4 (PM).

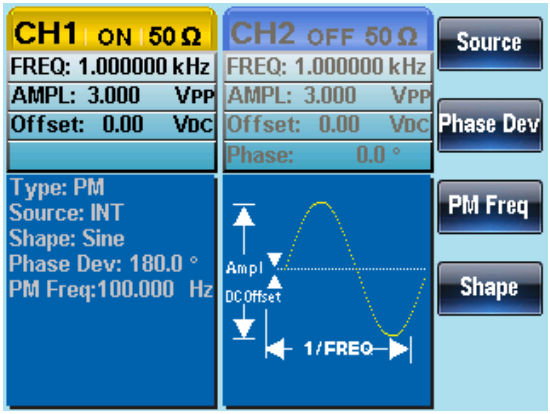

PM Carrier Waveform

Background PM uses a sine wave as default. Noise and Pulse waveform cannot be used with phase modulation.

Panel Operation

1. Press the Waveform key.

2. Press F1 ~ F4 to select the waveform.



Range	Carrier Waveform	Sine wave, Square wave, ramp wave.

PM Carrier Frequency

Selects the maxium carrier frequency for the carrier wavefrom. The default carrier frequency is 1kHz.

Panel Operation

1. Press the FREQ/Rate key to select the carrier frequency.

2. The FREQ parameter will become highlighted in the parameter window.

3. Use the arrow keys and scroll wheel or number pad to enter the carrier frequency.



4. Press F1~F5 to select the frequency unit.



Range	Carrier Wave	Carrier Frequency
	Sine wave	1μHz~25MH
	Square wave	1μHz~15MHz
	Ramp wave	1μHz~1MHz
	Default frequency	1 kHz

PM Wave Shape

The function generator can accept internal or external sources. The internal sources can include sine, square, triangle, up ramp and down ramp. The default wave shape is sine.

Panel Operation

1. Select the MOD key.

2. Press F4 (PM).

3. Press F4 (Shape).

4. Press F1~F5 to select a waveform shape.



5. Press Return to return to the previous menu.

Range	Waveform	
	Square wave	50% Duty Cycle
	Up Ramp	100% Symmetry
	Triangle	50% Symmetry
	Dn Ramp	0% Symmetry

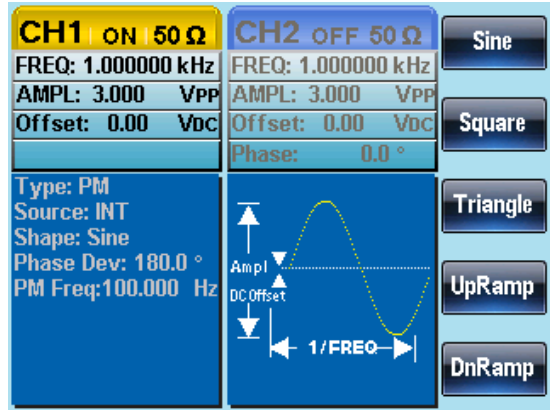

PM Frequency

The frequency of the modulation waveform (PM Frequency) can be set from 2mHz to 20kHz.

Panel Operation

1. Press the MOD key.

2. Press F4 (PM).

3. Press F3 (PM Freq).

4. The PM Freq parameter will become highlighted in the Waveform Display area.

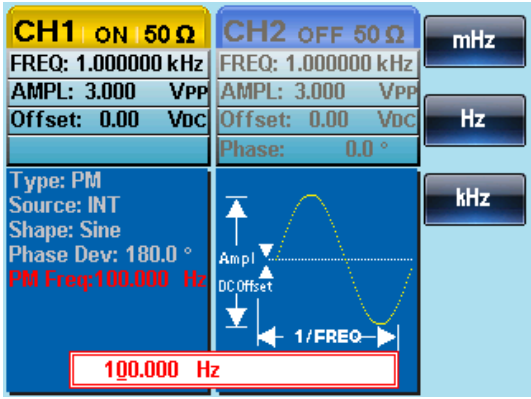

5. Use the arrow keys and scroll wheel or number pad to enter the PM frequency.



6. Press F1~F3 to select the frequency unit range.



Range	Modulation frequency	2mHz~20kHz
	Default frequency	100Hz

Phase Deviation

The maximum phase deviation depends on the the carrier wave frequency and the modulated waveform.

Panel operation

1. Press the MOD key.

2. Press F4 (PM).

3. Press F2 (Phase Dev).

4. The Phase Dev parameter will become highlighted in the waveform display area.

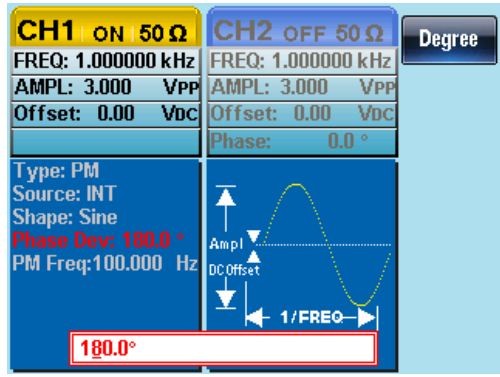

5. Use the arrow keys and scroll wheel or number pad to enter the phase deviation.



6. Press F1 to select the phase units.

Range	Phase deviation/shift	0~360°
	Defualt phase	180°

Select the PM Source

The function generator excepts internal or external sources for phase modulation. The default source is internal.

Panel Operation

1. Press the MOD key.

2. Press F4 (PM).

3. Press F1 (Source).

4. Press F1 (INT) or F2 (EXT) to select the source.



5. Press return to return to the previous menu.

External Source

Use the MOD INPUT terminal on the rear panel when using an external source.



Note

If the modulation source is set to external, the phase deviation is controlled by the ±5V MOD INPUT terminal on the rear panel. For example, if the modulation voltage is +5V, then the phase deviation is equal to the phase deviation setting. If the modulation voltage is less than +5V, then the phase deviation will be less than the phase deviation setting.

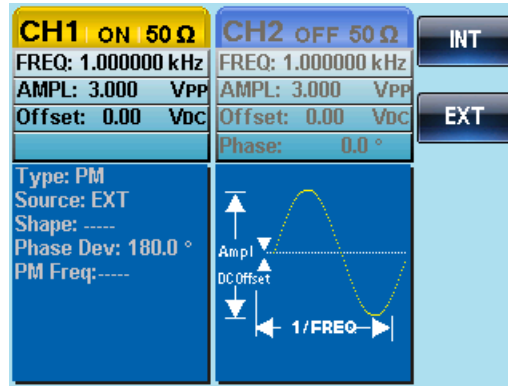
CH1 ON 50Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Type: PM
Source: EXT
Shape: -----
Phase Dev: 180.0 °
PM Freq:-----
CH2 OFF 50Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Phase: 0.0 °
Ampl
DC Offset
1/FREQ
INT
EXT

SUM modulation

Sum modulation adds a modulating signal to a carrier wave. Typically, sum modulation is used to add noise to a carrier wave. The modulating signal is added as a percentage of the carrier amplitude.

If SUM is enabled, any other modulation mode will be disabled. Likewise, burst and sweep modes cannot be used with SUM and will be disabled when SUM is enabled.

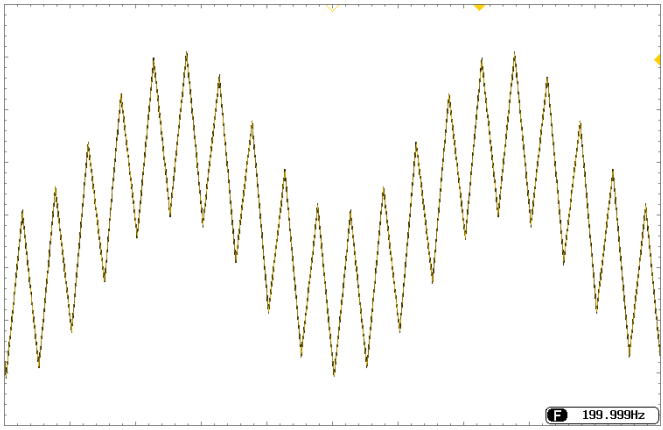

Selecting SUM modulation

For SUM modulation, the modulated waveform amplitude and offset is determined by the carrier wave.

Panel Operation

1. Press the MOD key.

2. Press F5 (SUM).

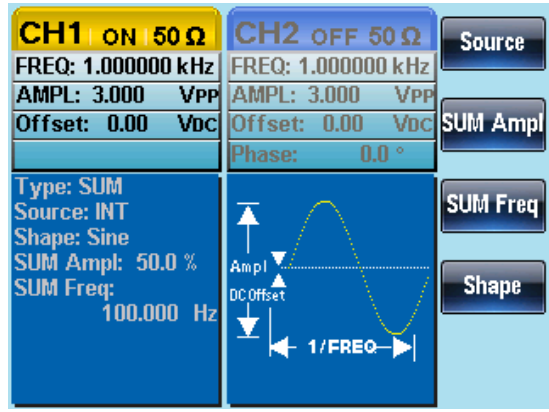

SUM Carrier Waveform

Background

The SUM carrier waveform is a sinewave by default.

Panel Operation

1. Press the Waveform key.

2. Press F1~F5 to select the carrier waveform.



Range	Carrier Waveform	Sine, square, pulse, ramp and noise wave.

SUM Carrier Frequency

The maximum carrier frequency depends on the selected carrier waveform. The default carrier frequency is 1kHz.

Panel Operation

1. Press the FREQ/Rate key to select the carrier frequency.

2. The FREQ parameter will become highlighted in the parameter window.

3. Use the arrow keys and scroll wheel or number pad to enter the frequency.



4. Press F1 ~ F5 to select the frequency units.



Range

Carrier Waveform	Carrier Frequency
Sine wave	1μHz~25MH
Square wave	1μHz~25MHz
Pulse wave	500μHz~25MHz
Ramp wave	1μHz~1MHz
Default frequency	1 kHz

SUM Waveform

The function generator can accept internal and external sources. The AFG-2225 includes sine, square, triangle, UpRamp and DnRamp as internal sources. The default waveform is sine.

Panel Operation

1. Press the MOD key.

2. Press F5 (SUM).

3. Press F4 (Shape).

4. Press F1~F5 to select the source waveform.



5. Press Return to return to the previous menu.

Range		
	Square wave	50% Duty cycle
	Up ramp	100% Symmetry
	Triangle	50% Symmetry
	Down ramp	0% Symmetry

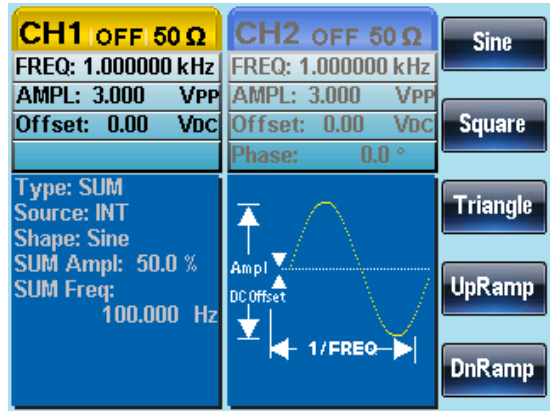

Modulating Waveform Frequency

The frequency of the modulating waveform (SUM Frequency) can be set from 2mHz to 20kHz.

Panel Operation

1. Press the MOD key.

2. Press F5 (SUM).

3. Press F3 (SUM Freq).

4. The SUM Freq parameter will become highlighted in the waveform display area.

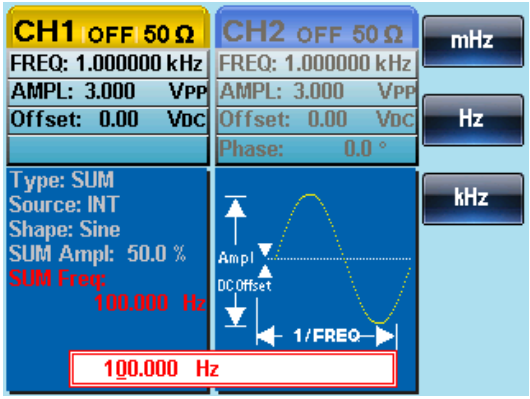

5. Use the arrow keys and scroll wheel or number pad to enter the SUM frequency.



6. Press F1~F3 to select the frequency units.



Range		
	Modulating range	2mHz~20kHz
	Default frequency	100Hz

SUM Amplitude

The SUM amplitude is the offset (in percent relative to the carrier) of the signal that is added to the carrier.

Panel Operation

1. Press the MOD key.

2. Press F5 (SUM).

3. Press F2 (SUM Ampl).

4. In the waveform display area, the SUM Ampl will be highlighted.

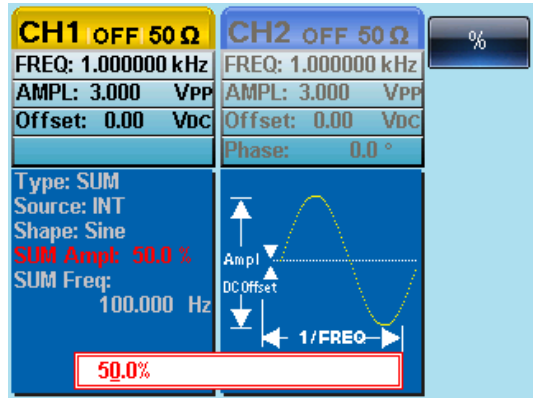

5. Use the arrow keys and scroll wheel or number pad to enter the SUM amplitude.



6. Press F1 to select the percentage unit.

Range		
	Sum amplitude	0~100%
	Default amplitude	50%

Select the SUM Amplitude Source

The signal generator can accept internal or external sources for the SUM amplitude modulation.

Panel Operation	1. Press the MOD key.	
	2. Press F5 (SUM).	
	3. Press F1 (Source).	
	4. Press F1 (INT) or F2 (EXT) to select the source.	
	5. Press Return to return to the previous menu.	
External Source	Use the MOD INPUT terminal on the rear panel when using an external source.	
Note	If an external modulation source is selected, the SUM amplitude is controlled by the ± 5V from the MOD INPUT terminal on the rear panel. For example, if the SUM amplitude is set to 0%, then the maximum amplitude (100% of the carrier) will be at +5V, and the minimum amplitude (0% of the carrier) will be at -5V.	

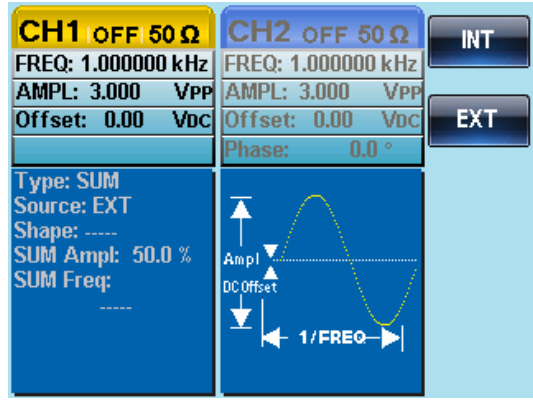
CH1 OFF 50 Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Type: SUM
Source: EXT
Shape: -----
SUM Ampl: 50.0 %
SUM Freq:

CH2 OFF 50 Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Phase: 0.0 °
Ampl
DC Offset
1/FREQ
INT
EXT

Frequency Sweep

The function generator can perform a sweep for sine, square or ramp waveforms, but not noise, and pulse. When Sweep mode is enabled, Burst or any other modulation modes will be disabled. When sweep is enabled, burst mode is automatically disabled.

In Sweep mode the function generator will sweep from a start frequency to a stop frequency over a number of designated steps. The step spacing of the sweep can linear or logarithmic. The function generator can also sweep up or sweep down in frequency. If manual or external sources are used, the function generator can be used to output a single sweep.

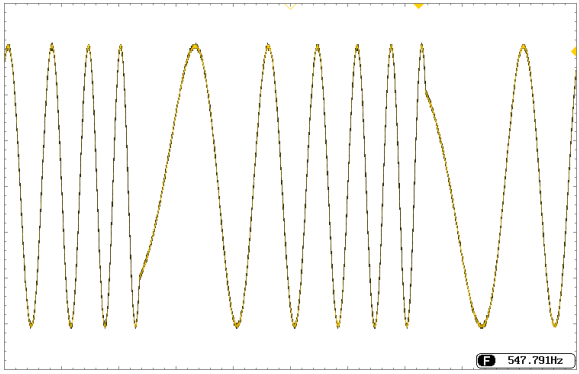

Selecting Sweep Mode

The Sweep button is used to output a sweep. If no settings have been configured, the default settings for output amplitude, offset and frequency are used.

Setting Start and Stop Frequency

The start and stop frequencies define the upper and lower sweep limits. The function generator will sweep from the start through to the stop frequency and cycle back to the start frequency. The sweep is phase continuous over the full range sweep range (1μHz-25MHz).

Panel Operation

1. Press the SWEEP key.

2. Press F3 (Start) or F4 (Stop) to selelect the start or stop frequency.



3. The Start or Stop parameter will become highlighted in the waveform display area.

Start

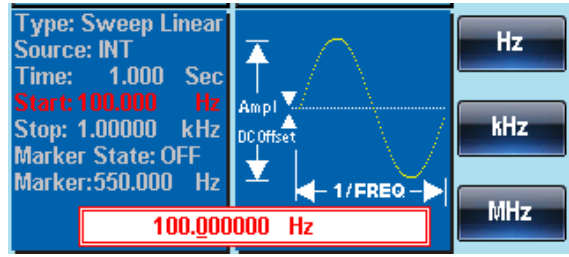

Stop

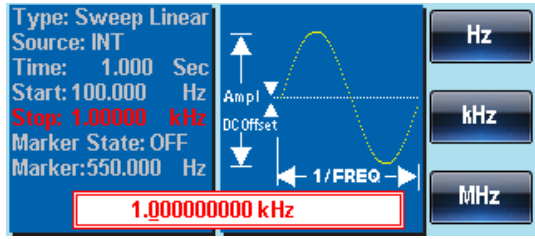

4. Use the arrow keys and scroll wheel or number pad to enter the Stop/Start frequency.



5. Press F1~F5 to select the Start/Stop frequency units.



Range	Sweep Range	1μHz~25MHz (Sine wave)
		1μHz~1MHz (Ramp wave)
		1μHz~15MHz (Square wave)
	Start - Default	100Hz
	Stop - Default	1kHz

Note

To sweep from low to high frequencies, set the start frequency less than the stop frequency.

When marker is on, the SYNC signal is at a TTL low level that rises to a TTL high level at the marker.

To sweep from high to low frequencies, set the start frequency greater than the stop frequency.

When marker is on, the SYNC signal is at a TTL high level that drops to a TTL low level at the marker.

When marker is off, the SYNC signal is turn off. The frequency of the SYNC signal is equal to the sweep time.

The SYNC signal is output from the trigger output terminal.

Center Frequency and Span

A center frequency and span can be set to determine the upper and lower sweep limits (start/stop).

Panel Operation

1. Press the SWEEP key.

2. Press F5 (More).

3. Press F2 (Span) or F3 (Center) to select the span or center.



4. The Span or Center parameters will become hightlighted in the waveform display area.

Span

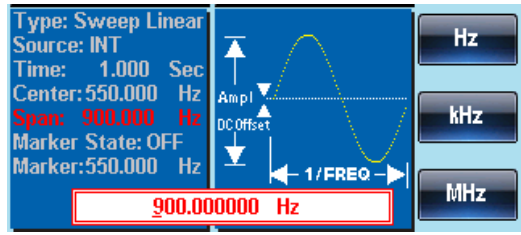

Center

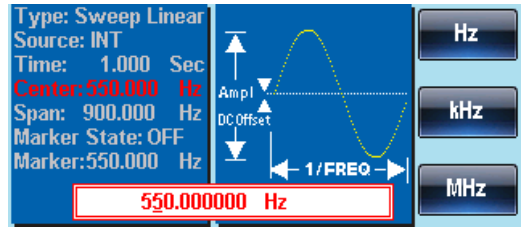

5. Use the arrow keys and scroll wheel or number pad to enter the Span/Center frequency.



6. Press F1~F5 to select the Start/Stop frequency units.



Range	Center frequency	1μHz~25MHz (sine wave) 1μHz~1MHz (Ramp wave) 1μHz~15MHz (square wave)
	Span frequency	DC~+/-25MHz (sine wave) DC ~+/-1MHz (Ramp wave) +/-1μHz~+/-15MHz (square wave)
	Default center	550Hz
	Default span	900Hz

Note

To sweep from low to high frequencies, set a positive span.

To sweep from high to low frequencies, set a negative span.

Sweep Mode

Sweep mode is used to select between linear or logarithmic sweeping. Linear sweeping is the default setting.

Panel Operation

1. Press the SWEEP key.

2. Press F2 (Type).

3. To select linear or logarithmic sweep, press F1 (Linear) or F2 (Log).



4. Press Return to return to the previous menu.

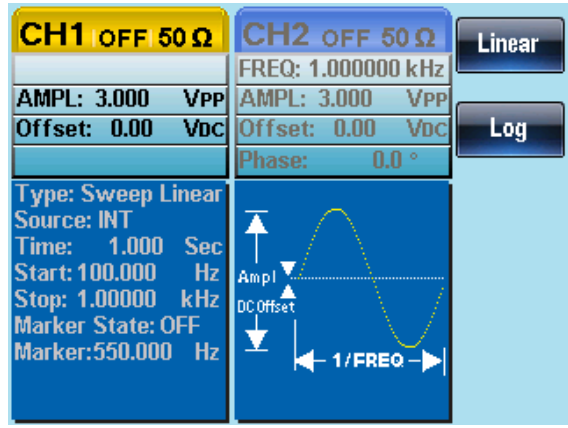

Sweep Time

The sweep time is used to determine how long it takes to perform a sweep from the start to stop frequencies. The function generator automatically determines the number of discrete frequencies used in the scan depending on the length of the scan.

Panel Operation

1. Press the SWEEP key.

2. Press F5 (More).

3. Press F1 (SWP Time).

4. The Time parameter will become highlighted in the waveform display area.

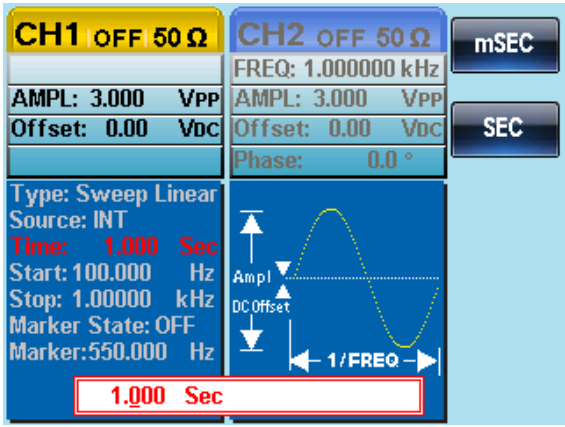

5. Use the selector keys and scroll wheel or number pad to enter the Sweep time.



6. Press F1~F2 to select the time unit.



Range	Sweep time	1ms ~ 500s
	Default time	1s

Marker Frequency

The marker frequency is the frequency at which the marker signal goes low /high(The marker signal is high/low at the start of each sweep). The marker signal is output from the Trigger OUT terminal on the rear panel. The default is 550 Hz.

Panel Operation

1. Press the SWEEP key.

2. Press F5 (More).

3. Press F4 (Marker)

4. Press F2 (ON/OFF) to toggle the marker on or off.

5. Press F1 (Freq) to select the marker frequency.

6. The Marker parameter will become highlighted in the waveform display area.

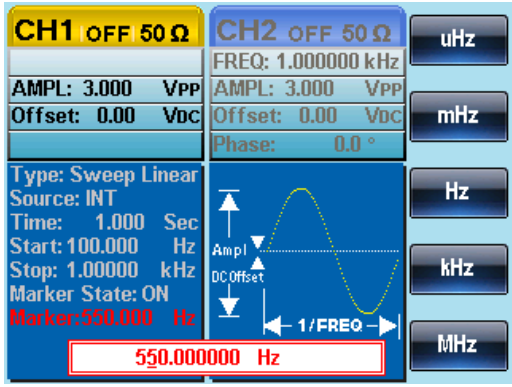

7. Use the arrow keys and scroll wheel or number pad to enter the frequency.



8. Press F1~F5 to select the frequency unit.



Range	Frequency	1μHz~25MHz(Sine wave) 1μHz~1MHz (Ramp wave) 1μHz~15MHz(square wave)
	Default	550Hz

Note

The marker frequency must be set to a value between the start and stop frequencies. If no value is set, the marker frequency is set to the average of the start and stop frequencies.

Marker mode will override SYNC mode settings when sweep mode is active.

Sweep Trigger Source

In sweep mode the function generator will sweep each time a trigger signal is received. After a sweep output has completed, the function

generator outputs the start frequency and waits for a trigger signal before completing the sweep. The default trigger source is internal.

Panel Operation

1. Press the SWEEP key.

2. Press F1 (Source).

3. To select the trigger source, press F1 (Internal), F2 (External) or F3 (Manual).



4. Press Return to return to the previous menu.

Note

Using the Internal source will produce a continuous sweep using the sweep time settings.

With an external source, a sweep is output each time a trigger pulse (TTL) is received from the Trigger IN terminal on the rear panel.

The trigger period must be equal to or greater than the sweep time plus 1ms.

5. If manual is selected, press F1 (Trigger) to manually start each sweep.

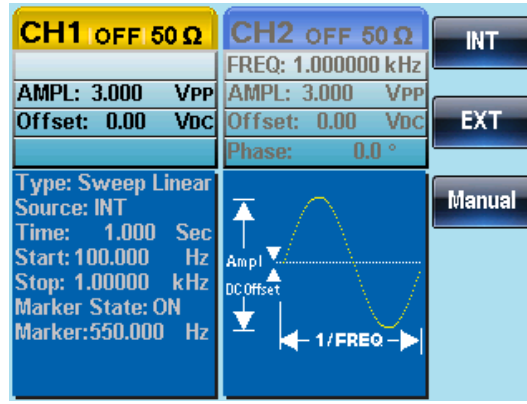

Burst Mode

The function generator can create a waveform burst with a designated number of cycles. Burst mode supports sine, square ,ARB and ramp waveforms.

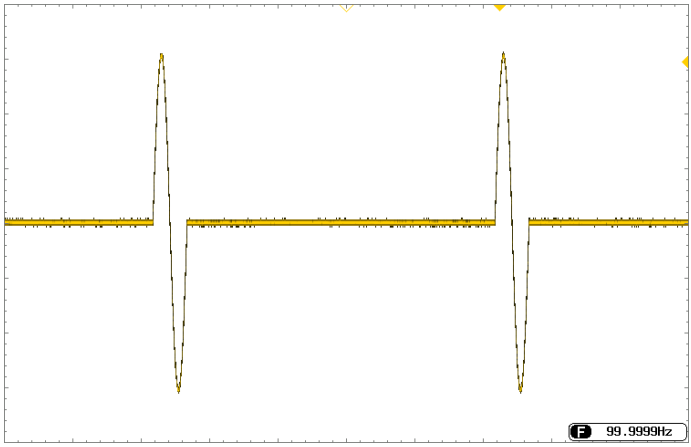

Selecting Burst Mode

When burst mode is selected, any modulation or sweep modes will be automatically disabled. If no settings have been configured, the default settings for output amplitude, offset and frequency are used.

Burst Modes

Burst mode can be configured using Triggered (N Cycle mode) or Gated mode. Using N Cycle/Triggered mode, each time the function generator receives a trigger, the function generator will output a specified number of waveform cycles (burst). After the burst, the function generator will wait for the next trigger before outputting another burst. N Cycle is the default Burst mode. Triggered mode can use internal or external triggers.

The alternative to using a specified number of cycles, Gated mode uses the external trigger to turn on or off the output. When the Trigger INPUT signal is high, waveforms are continuously output. When the Trigger INPUT signal goes low, the waveforms will stop being output after the last waveform completes its period. The voltage level of the output will remain equal to the starting phase of the burst waveforms, ready for the signal to go high again.

Burst Mode	Burst Count	Burst Period	Phase	Trigger Source
Triggered (Int)	Available	Available	Available	Immediate
Triggered (Ext)	Available	Not used	Available	EXT, Bus
Gated pulse (Ext)	Not used	Not used	Available	Unused

In Gated mode, burst count, burst cycle and trigger source are ignored. If a trigger is input, then the trigger will be ignored and will not generate any errors.

Panel Operation

1. Press the Burst key.

2. To select either N Cycle (F1) or Gate (F2).



Burst Frequency

In the N Cycle and Gated modes, the waveform frequency sets the repetition rate of the burst waveforms. In N-Cycle mode, the burst is output at the waveform frequency for the number of cycles set. In Gated mode the waveform frequency is output while the trigger is high. Burst mode supports sine, square ,ARB or ramp waveforms.

Panel Operation

1. Press the FREQ/Rate key.

2. The FREQ parameter will become highlighted in the parameter window.

3. Use the arrow keys and scroll wheel or number pad to enter the frequency.



4. Press F1~F5 to select the frequency unit.



Range	Frequency_sine	1uHz~15MHz
	Freqency – Ramp	1uHz~1MHz
	Freqency – Square	1uHz~15MHz
	Default	1kHz

Note Waveform frequency and burst period are not the same. The burst period is the time between the bursts in N-Cycle mode.

Burst Cycle/Burst Count

The burst cycle (burst count) is used to define the number of cycles that are output for a burst waveform. Burst cycle is only used with N-cycle mode (internal, external or manual source). The default burst cycle is 1.

Panel Operation

1. Press the Burst key.

2. Press F1 (N Cycle).

3. Press F1 (Cycles).

4. The Cycles parameter will become highlighted in the Waveform Display area.

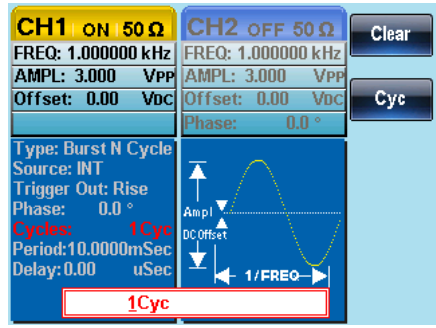

5. Use the arrow keys and scroll wheel or number pad to enter the number of cycles.



6. Press F2 to select the Cyc unit.

Range	Cycles	1~65535

Note

Burst cycles are continuously output when the internal trigger is selected. The burst period determines the rate of bursts and the time between bursts.

Burst cycle must be less than the product of the burst period and wave frequency.

Burst Cycle < (Burst Period x Wave Frequency)

If the burst cycle exceeds the above conditions, the burst period will be automatically increased to satisfy the above conditions.

If gated burst mode is selected, burst cycle is ignored. Though, if the burst cycle is changed remotely whilst in gated mode, the new burst cycle is remembered when used next.

Infinite Burst Count

Panel Operation

1. Press the Burst key.

2. Press F1 (N Cycle).

3. Press F2 (Infinite).

Note: Infinite burst is only available when using manual triggering.

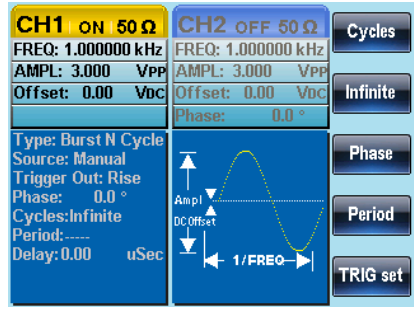

Burst Period

The burst period is used to determine the time between the start of one burst and the start of the next burst. It is only used for internally triggered bursts.

Panel Operation

1. Press the Burst key.

2. Press F1 (N Cycle).

3. Press F4 (Period).

4. The Period parameter will become highlighted in the Waveform Display area.

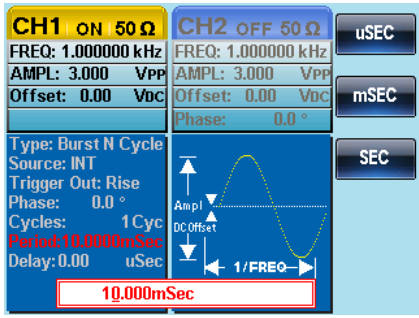

5. Use the arrow keys and scroll wheel or number pad to enter period time.



6. Press F1~F3 to choose the period time unit.



Range	Period time	1ms~500s
	Default	10ms

Note

Burst period is only applicable for internal triggers. Burst period settings are ignored when using gated burst mode or for external and manual triggers.

The burst period must be large enough to satisfied the condition below:

Burst Period>Burst Count/Wave frequency + 200ns.

Burst Phase

Burst Phase defines the starting phase of the burst waveform. The default is 0˚.

Panel Operation

1. Press the Burst key.

2. Press F1 (N Cycle).

3. Press F3 (Phase).

4. The Phase parameter will become highlighted in the Waveform Display area.

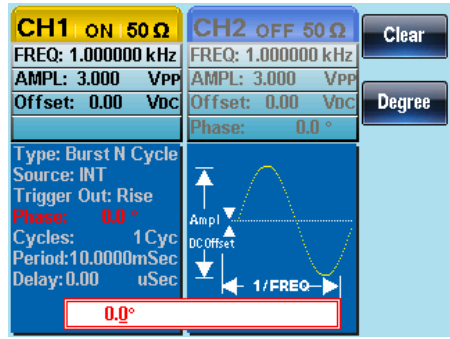

5. Use the arrow keys and scroll wheel or number pad to enter the phase.



6. Press F2 (Degreee) to select the phase unit.

Range	Phase	-360˚~+360˚
	Default	0˚

Note

When using sine, square, triangle or ramp waveforms, 0˚ is the point where the waveforms are at zero volts.

0˚ is the starting point of a waveform. For sine, square or Triangle, Ramp waveforms, 0˚ is at 0 volts (assuming there is no DC offset).

Burst Phase is used for both N cycle and Gated burst modes. In gated burst mode, when the Trigger INPUT signal goes low the output is stopped after the current waveform is finished. The voltage output level will remain equal to the voltage at the starting burst phase.

Burst Trigger Source

Each time the function generator receives a trigger in triggered burst (N-Cycle) mode, a waveform burst is output. The number of waveforms in each burst is designated by the burst cycle (burst count). When a burst has completed, the function generator waits for the next trigger. Internal source is the default triggered burst (N-cycle) mode on power up.

Panel Operation

1. Press the Burst key.

2. Press F1 (N Cycle).

3. Press F5 (TRIG set).

4. Choose a trigger type by pressing F1 (INT), F2 (EXT) or F3 (Manual).



Manual Triggering

If a manual source is selected, the Trigger softkey (F1) must be pressed each time to output a burst.

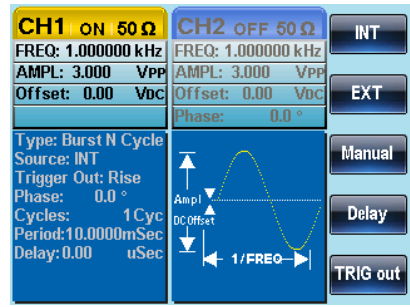

Note

When the internal trigger source is chosen, the burst is output continuously at a rate defined by the burst period setting. The interval between bursts is defined by the burst period.

When the external trigger is selected the function generator will receive a trigger signal (TTL) from the Trigger INPUT terminal on the rear panel. Each time the trigger is received, a burst is output (with the defined number of cycles). If a trigger signal is received during a burst, it is ignored.

When using the manual or external trigger only the burst phase and burst cycle/count are applicable, the burst period is not used.

A time delay can be inserted after each trigger, before the start of a burst.

Burst Delay

Panel Operation

1. Press the Burst key.

2. Press F1 (N Cycle).

3. Press F5 (TRIG set).

4. Press F4 (Delay).

5. The Delay parameter will become highlighted in the Waveform Display area.

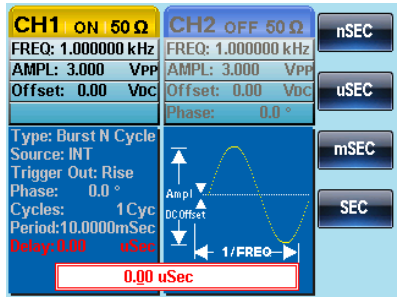

6. Use the selector keys and scroll wheel or number pad to enter period time.



7. Press F1~F4 to choose the delay time unit.



Range	Delay time	0s~655350nS
	Default	0s

Burst Trigger Output

The Trig Out terminal on the rear panel can be used for burst or sweep modes to output a rising edge TTL compatible trigger signal. By default the trigger signal is rising edge. The trigger signal is output at the start of each burst.

Panel Operation

1. Press the Burst key.

2. Press F1 (N Cycle).

3. Press F5 (TRIG set).

4. Press F5 (TRIG out).

5. Press F3 (ON/OFF) to toggle Trigger out ON/OFF.

6. Select F1 (Rise) or F2 (Fall) edge trigger.



Note

When the internal or external trigger is selected, the trigger output signal will be at either a TTL low/high level and will toggle.when the specifed number of waveform cycles completed.

When the manual trigger is selected, the trigger output turns on at the trigger soft-key be pressed.

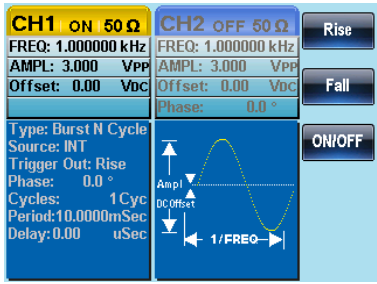
CH1 ON 50Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Type: Burst N Cycle
Source: INT
Trigger Out: Rise
Phase: 0.0 °
Cycles: 1 Cyc
Period: 10.0000mSec
Delay: 0.00 uSec
CH2 OFF 50Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Phase: 0.0 °
Ampl
DC Offset
1/FREQ
Rise
Fall
ON/OFF

SECONDARY SYSTEM FUNCTION SETTINGS

The secondary system functions are used to store and recall settings, view help files, view the software version, update the firmware, set the buzzer.

Save and Recall 132
System and Settings 136
System and Settings 136
Viewing and Updating the Firmware 136
Setting the Buzzer Sound 137

Save and Recall

The AFG-2225 has non-volatile memory to store instrument state and ARB data. There are 10 memory files numbered 0~9. Each memory file can either store arbitrary waveform data (ARB), settings or both. When data (ARB or Setting data) is stored in a memory file, the data will be shown in red. If a file has no data, it will be shown in blue.

Save/Recall Properties

ARB

- Rate
- Frequency
- Length
- Display horizontal
- Display vertical
- Output Start
- Output length

Setting

- Functions
  - Waveform
  - Frequency
  - Pulse Width
  - Square wave Duty
  - Ramp Symmetry
  - Amplitude
  - Amplitude unit
  - Offset
  - Modulation type
  - Beep setting
  - Impedance
  - Main output
- Sweep
  - Source
  - Type
  - Marker
- AM
  - Source
  - Shape
  - Depth
  - AM frequency
- FM
  - Source
  - Shape
  - Deviation
  - FM frequency
- FSK
  - Source
  - Shape
  - Rate
  - Hop frequency
- PM
  - Source

- Time
- Start frequency
- Stop frequency
- Center frequency
- Span frequency
- Marker frequency
- Shape
- Phase deviation
- Frequency
- Burst Type
  - Source
  - Trigger out
  - Type
  - Cycles
  - Phase
  - Period
  - Delay

Panel Operation

1. Press the UTIL key.

2. Press F1 (Memory).

3. Use the scroll wheel to highlight a memory file number.



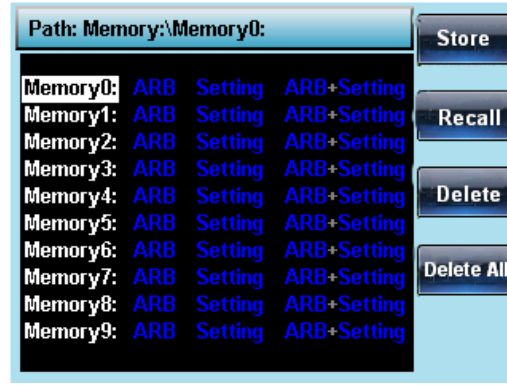

4. Choose a file operation:

   Press F1 to store a file, press F2 to recall a file, or press F3 to delete a file.

5. Use the scroll wheel to highlight the data type.

   ARB, Setting or ARB+Setting



6. Press F5 (Done) to choose the data type.

Range	Memory file	Memory0 ~ Memory9
	Data type	ARB, Setting, ARB+Setting

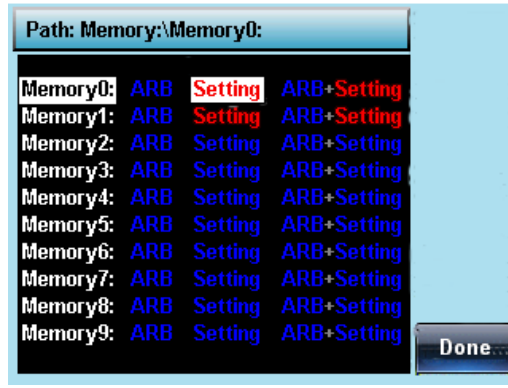

7. Press F5 (Done) to confirm the operation.

Delete All

8. To delete all the files for Memory0~Memory9, press F4.

9. Press F1 (Done) to confirm the deletion of all files.

System and Settings

There are a number of miscellaneous settings and firmware settings that can be configured.

Viewing and Updating the Firmware

View Version	1. Press the UTIL key.	
	2. Press F2 (Cal.).	
	3. Press F2 (Software).	
	4. Press F1 (Version) to view the firmware version.	
	The version information will be shown on screen: Instrument, Version, FPGA Revision	
Update Firmware	5. To update the firmware, insert a USB flash drive with a firmware file in the USB host drive. Press F2 (Upgrade).	
Note	The firmware file (*.bin) must be located in a directory, directly off the USB root directory.	

Setting the Buzzer Sound

Background — Turns the beeper on or off.

Panel Operation

1. Press the UTIL key.

2. Press F3 (System).

3. PressF3 (Beep) to toggle the buzzer sound on or off.

4. Press F1(ON) or Press F2(OFF)



Frequency Counter

Example: Turn on the frequency counter. Gate time: 1 second.

Output: N/A

Input:



1. Press UTIL, F5 (Counter).

2. Press F1 (Gate Time), and press F3 (1 Sec) to choose a gate time of 1 second.

3. Connect the signal of interest to the Frequency counter input on the rear panel.

4. Input a 1kHz square wave signal into the Counter input on the rear panel. Set the gate time to 1S.

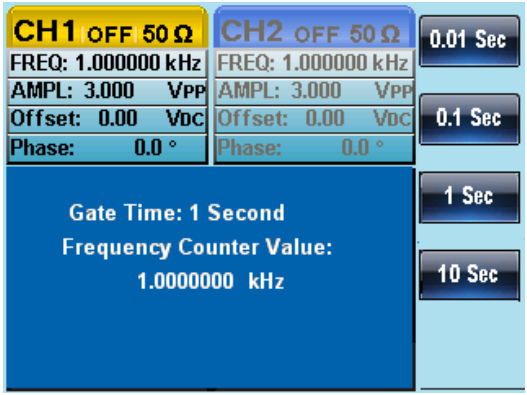

Frequency Coupling

Example: Frequency Coupling

1. Press UTIL, F4 (Dual Chan) to enter the coupling function.

2. Press F1 (Freq Cpl) to select the frequency coupling function.

3. Press F2 (Offset). The offset is the frequency difference between CH1 and CH2. Use the number keys or scroll wheel to enter the offset.

   There are two different coupling modes. They are calculated as follows:

   Offset=CH2-CH1

   Ratio=CH2/CH1

4. Input an offset value of 1kHz. Press F1~ F5 to select the units.



The frequency of channel 2 becomes 2kHz (CH2=CH1 + Offset).

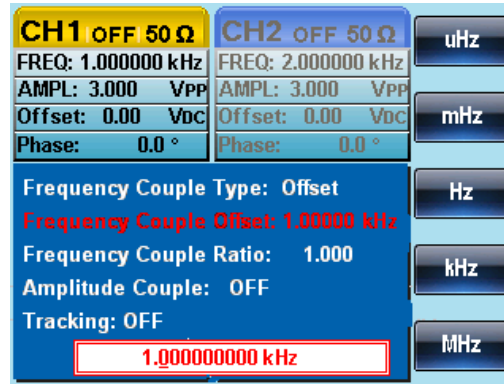

5. Change the frequency coupling mode to Ratio. Set the ratio to 2.

   The frequency of CH2 automatically changes accordingly to match the ratio (CH2=CH1*Ratio).

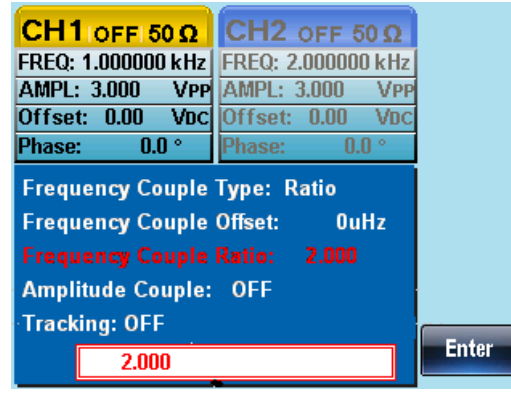

Amplitude Coupling

Example: Amplitude Coupling

1. The following assumes that the amplitude has already been set to 4Vpp with a DC offset of 1Vdc.

2. Press UTIL, F4 (Dual Chan) to enter the coupling function.

3. Press F2 (Ampl Cpl), F1 (ON) to select the amplitude coupling function.

4. The amplitude and offset between both channel is coupled. Any changes in amplitude in the current channel is reflected in the other channel.

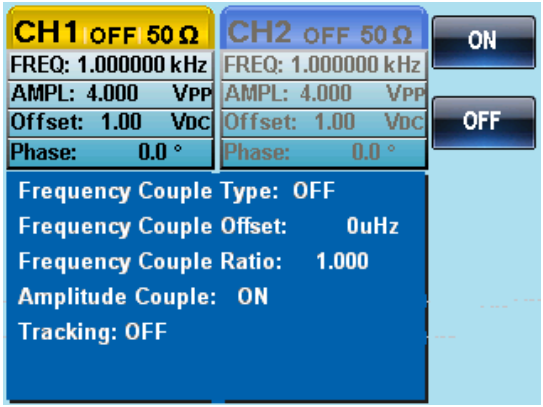

Tracking

Example: Tracking

1. The method for outputting a square wave has been previously described. Use this method to output a 2kHz squarewave from CH1 with an amplitude of 5Vpp and a DC offset of 1Vdc.

2. Press UTIL, F4 (Dual Chan) to enter the coupling function.

3. Press F3 (Tracking), F2 (On) to turn on the tracking function.

4. When tracking is turned on, parameters such as amplitude and frequency from the current channel are mirrored on the other channel.

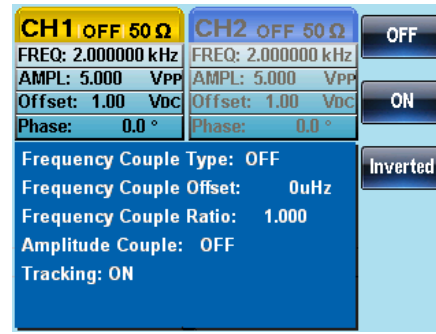

S_Phase

Example: S_phase

5. Press UTIL, Dual Chan (F4) to enter the coupling function.

2. Press S_Phase (F4), turn on the S_Phase function.

3. S_Phase function is to make the phase synchronization between current channel and another channel. Phase is 0° .here S_Phase function is the same with S_Phase function under CH1/CH2.

CHANNEL SETTINGS

The channel settings chapter shows how to set the output impedance, output phase and DSO connection settings.

Output Impedance 143
Selecting the Output Phase 144
Synchronizing the Phase 145
DSO Link 146

Output Impedance

Background

The AFG-2225 has selectable output impedances: 50Ω or high impedance. The default output impedance is 50Ω. The output impedances are to be used as a reference only. If the actual load impedance is different to that specified, then the actual amplitude and offset will vary accordingly.

Panel Operation

1. Press the CH1/CH2 key. 

Note

The load function can only be used if the ARB, MOD, SWEEP or BURST functions are not active.

2. Press F1 (Load).

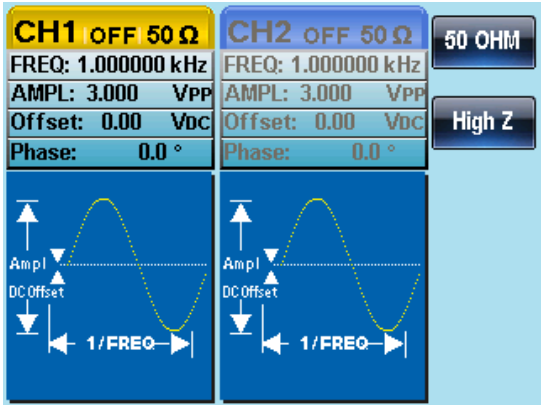

3. Select F1 (50 OHM) or F2 (High Z) to select the output impedance.



Selecting the Output Phase

Panel operation

1. Press the CH1/CH2 key.

Note

The phase function can only be used if the ARB, MOD, SWEEP or BURST functions are not active. Square and Pulse can not be change,phase is 0°

2. Press F4 (Phase) and then press F1 (Phase)

3. The Phase parameter in the parameter window will become hightlighed.

4. Use the arrow keys and scroll wheel or number pad to enter the output phase.



5. Press F5 (Degree).

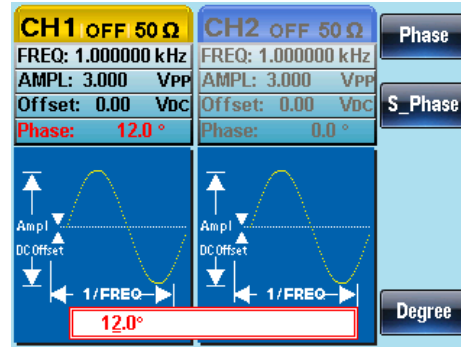

Synchronizing the Phase

Background — Synchronizes both the outputs on the AFG-2225.

Panel Operation

1. Press the CH1/CH2 key.



2. Press F4 (Phase).

3. Press F2 (S_Phase) to synchronize the phase of the channels.

DSO Link

Background

DSO Link enables the AFG-2225 to receive lossless data from a GDS-2000 Series DSO to create ARB data.

1. Connect the AFG-2225 USB host port to the GDS-2000's USB B device port.



Panel Operation

2. Press the CH1/CH2 key.



3. Press F5 (DSO Link).

4. Press F1 (Search).

5. To select a DSO channel, Press F2 (CH1), F3 (CH2), F4 (CH3) or F5 (CH4). The acquired data can then be displayed.



ARBITRARY WAVEFORMS

The AFG-2225 can create user-defined arbitrary waveforms with a sample rate of 120MHz. Each waveform can include up to 4k of data points with a vertical range of ±511.

Inserting Built-In Waveforms 148
Create an AbsAtan Waveform 148
Display an Arbitrary Waveform 150
Set the Horizontal Display Range 150
Set the Vertical Display Properties 152
Page Navigation (Back Page) 154
Page Navigation (Next Page) 156
Display 158
Editing an Arbitrary Wavefrom 159
Adding a Point to an Arbitrary Waveform 159
Adding a Line to an Arbitrary Waveform 160
Copy a Waveform 162
Clear the Waveform 164
ARB Protection 166
Ouput an Arbitrary Waveform 169
Ouput Arbitrary Waveform 169
Saving/Loading an Arbitrary Waveform 171
Saving a Waveform to Internal Memory 171
Saving a Waveform to USB Memory 172
Load a Waveform from Internal Memory 175
Load a Waveform from USB 178

Inserting Built-In Waveforms

The AFG-2225 includes 66 common waveforms, such as math waveforms, windowing functions and engineering waveforms.

Create an AbsAtan Waveform

Panel Operation

1. Press the ARB key.

2. Press F3(Built in).

3. Press F4(Wave).

4. Press F1(Common).

5. Use the scroll wheel to select "AbsAtan" from the built-in Common waveforms.

6. Press F5(Select) to select AbsAtan waveform

7. Press F1(Start) and set the start position of the AbsAtan waveform.

8. You can also change the length and scale of the waveform by pressing F2(Length) or F3(Scale).

9. Press F5 (Done) to complete the operation

10. Press return to return to the previous menu.

Below an Absatan wave created at start:0, Length: 33, Scale: 511

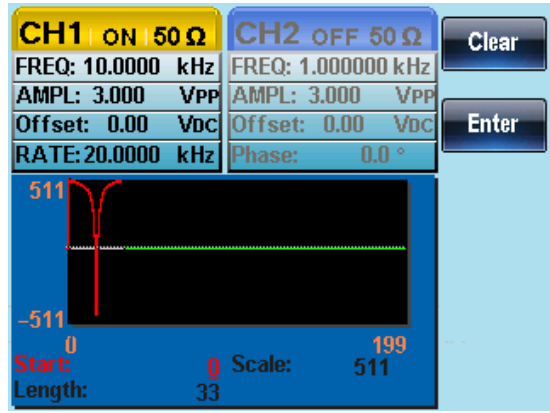

*Please see the appendix for other built-in waveforms

Display an Arbitrary Waveform

Set the Horizontal Display Range

The horizontal window bounds can be set in one of two ways: Using a start point and length, or a center point and length.

Panel Operation

1. Press the ARB key.

2. Press F1 (Display) to enter the display menu.

3. Press F1 (Horizon) to enter the horizontal menu.

Using a Start Point

4. Press F1(Start)

5. The H_From parameter will become highlighted.

6. Use the arrow keys and scroll wheel or number pad to enter the H_From value.



7. Press Clear (F1) to cancel.

8. Press F2 (Enter) to save the settings.

9. Press Return to return to the previous menu.

Setting the Length	10. Repeat steps 4~9 for Length (F2).	Length F2
Using a Center Point	11. Repeat steps 4~9 for Center (F3).	Center F3
Zoom in	12. To zoom into the arbitrary waveform, press F4 (Zoom In). The Zoom In function will reduce the length by half each time the function is used. The minimum allowable length is 3.	Zoom In F4
Zoom out	13. To zoom out from the center point of the waveform, press F5 (Zoom out). The Zoom out function will increase the length by 2. The maximum allowable length is 4096.	Zoom out F5

Below, an arbitrary waveform has a start of 0, length of 200 and is centered at 100.

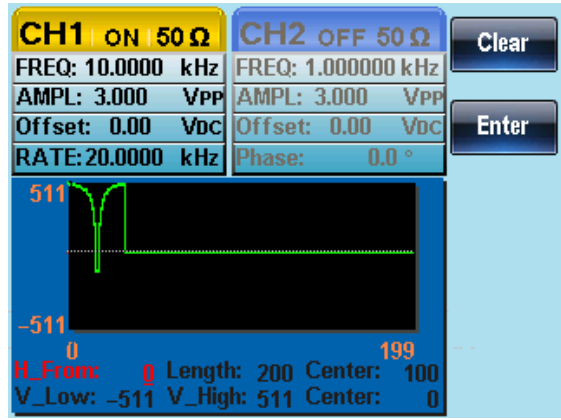

Set the Vertical Display Properties

Like the horizontal properties, the vertical display properties of the waveform display can be created in two ways: Setting high and low values, or setting the center point.

Panel Operation	1. Press the ARB key.	
	2. Press F1 (Display).	
	3. Press F2 (Vertical).	
Setting the Low Point	4. Press F1 (Low).	
	5. The V_Low parameter will become highlighted.	
	6. Use the arrow keys and scroll wheel or number pad to enter the V_Low value.	
	7. Press Clear (F1) to cancel.	
	8. Press F2 (Enter) to save the settings.	
	9. Press Return to return to the previous menu.	
Setting the High Point	10. Repeat steps 4~9 for V_High (F2).	

Setting the Center Point

11. Repeat steps 4~9 for Center (F3).

Zoom

12. To zoom in from the center of the arbitrary waveform, press F4 (Zoom in). The Zoom in function will reduce the length by half each time the function is used. The minimum allowable vertical low is -2, and the minimum vertical high is 2.

13. To zoom out of the waveform, press F5 (Zoom out). The Zoom out function will increase the length by 2. The Vertical low maximum can be set to -511 and the vertical high maximum can be set to +511.

Below, the AbsAtan wave is with a vertical low of -511, a vertical high 511 and a center of 0.

Page Navigation (Back Page)

Background

When viewing the waveform, the display window can be moved forward and backward using the Next/Back Page functions.

Panel Operation

1. Press the ARB key.

2. Press F1 (Display).

3. Press F4 (Back Page) to move the display window one view length backward.

H_From* = H_From - Length
Center*= Center – Length
*Length until 0

Below, shows the display after Back Page has been pressed.

H_From: 200 → 0
Length: 200
Center:300→ 100

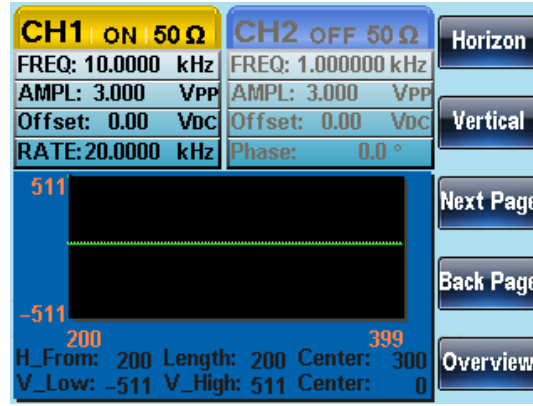
CH1 ON 50Ω
FREQ: 10.0000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
RATE: 20.0000 kHz
CH2 OFF 50Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Phase: 0.0 °
511
-511
200
399
H_From: 200 Length: 200 Center: 300
V_Low: -511 V_High: 511 Center: 0
Horizon
Vertical
Next Page
Back Page
Overview

CH1 OFF 50Ω
FREQ: 10.0000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
RATE: 20.0000 kHz
CH2 OFF 50Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Phase: 0.0 °
511
-511
0
4095
H_From: 0 Length: 4096 Center: 2048
V_Low: -511 V_High: 511 Center: 0
Horizon
Vertical
Next Page
Back Page
Overview

Page Navigation (Next Page)

Background

When viewing the waveform, the display window can be moved forward and backward using the Next/Back Page functions.

Panel Operation

1. Press the ARB key.

2. Press F1 (Display).

3. Press F3 (Next Page) to move the display window one view length forward.

H_From*＝H_From + Length
Center=Center + Length
*H_From +Length ≤ 4096

Below, shows the display after Next Page has been pressed.

H_From: 0 → 200
Length: 200
Center:100→ 300

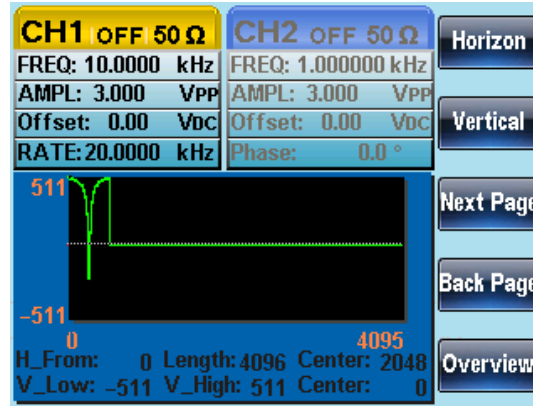
CH1 OFF 50Ω
FREQ: 10.0000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
RATE: 20.0000 kHz
CH2 OFF 50Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Phase: 0.0 °
511
-511
0
4095
H_From: 0 Length: 4096 Center: 2048
V_Low: -511 V_High: 511 Center: 0
Horizon
Vertical
Next Page
Back Page
Overview

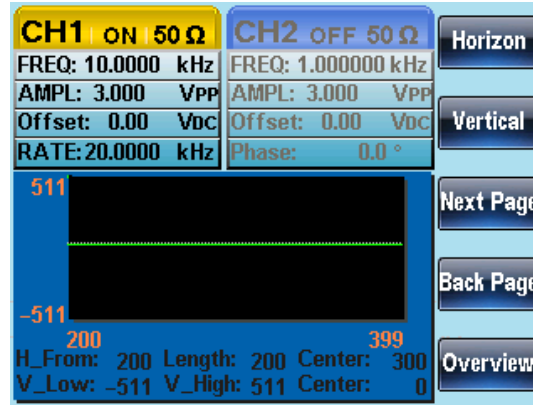
CH1 ON 50Ω
FREQ: 10.0000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
RATE: 20.0000 kHz
CH2 OFF 50Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Phase: 0.0 °
511
-511
200
399
H_From: 200 Length: 200 Center: 300
V_Low: -511 V_High: 511 Center: 0
Horizon
Vertical
Next Page
Back Page
Overview

Display

Panel Operation

1. Press the ARB key.

2. Press F1 (Display).

3. To make the display window cover the whole waveform, press F5 (Overview).

Horizontal: 0~4095
Vertical: 511~ -511

Below shows the display after Overview has been selected.
H_From: 0 → 0
Length: 400→4096
Center:200→ 2048
Vertical low/high: ±511

Editing an Arbitrary Wavefrom

Adding a Point to an Arbitrary Waveform

Background

The AFG-2225 has a powerful editing function that allows you to create points or lines anywhere on the waveform.

Panel Operation

1. Press the ARB key.

2. Press F2 (Edit).

3. Press F1 (Point).

4. Press F1 (Address).

5. The Address parameter becomes highlighted.

6. Use the arrow keys and scroll wheel or number pad to enter the Address value.



7. Press F2 (Enter) to save the settings.

8. Press Return to return to the previous menu.



9. Press F2 (Data).

10. The Data parameter will become highlighted.

11. Use the selector keys and scroll wheel or number pad to enter a Data value.



12. Press F2 (Enter) to save the settings.

13. Press Return to return to the previous menu.

14. Press return again to go back to the ARB menu.

In the following figure the edited address is shown in red.

Address 100， Data 200

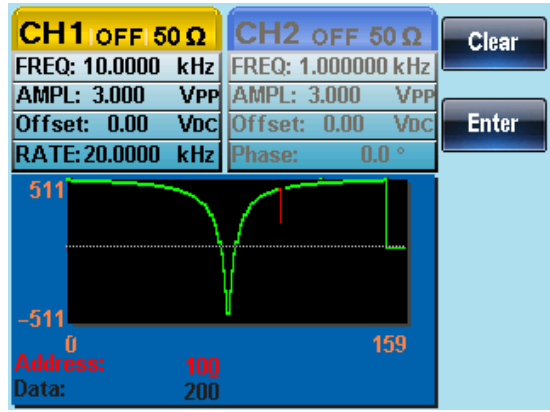

Adding a Line to an Arbitrary Waveform

Background

The AFG-2225 has a powerful editing function that allows you to create points or lines anywhere on the waveform.

Panel Operation

1. Press the ARB key.

2. Press F2 (Edit).

3. Press F2 (Line).

4. Press F1 (Start ADD).

5. The Start Address parameter will be highlighted in red.

6. Use the arrowkeys keys and scroll wheel or number pad to enter the start address.



7. Press F2 (Enter) to save the settings.

8. Press Return to return to the previous menu.

9. Repeat steps 4~8 for Start Data (F2), Stop Address (F3) and Stop Data (F4).

10. Press F5 (Done) to confirm the line edit.

11. Press Return to return to the previous menu.

The red line was created below with the following properties:

Start Address: 0, Start Data: 0
Stop Address: 32, Stop Data: 0

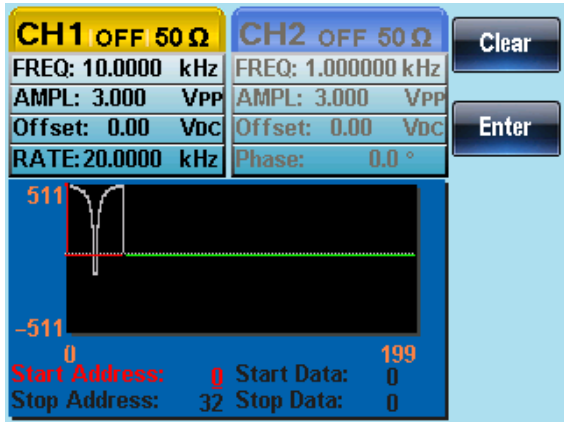

Copy a Waveform

Panel Operation

1. Press the ARB key.

2. Press F2 (Edit).

3. Press F3 (Copy).

4. Press F1 (Start).

5. The Copy From properties will become highlighted in red.

6. The the arrow keys and scroll wheel or number pad to enter the Copy From address.



7. Press F2 (Enter) to save the settings.

8. Press Return to return to the previous menu.

9. Repeat steps 4~8 for Length (F2) and Paste To (F3).

10. Press F5 (Done) to confirm the selection.

11. Press Return to return to the previous menu.

A section of the waveform from points 0~33 was copied to points 50~83:

Copy From: 0
Length: 33
To: 50

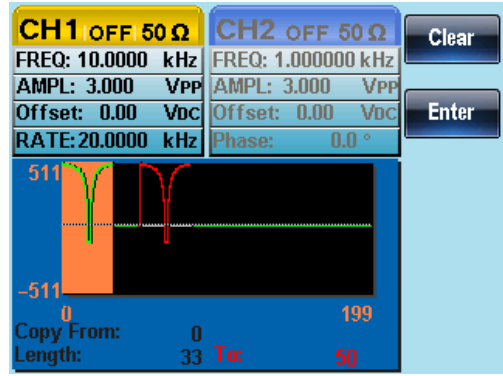

Clear the Waveform

Panel Operation

1. Press the ARB key.

2. Press F2 (Edit).

3. Press F4 (Clear).

4. Press F1 (Start).

5. The Clear From properties will become highlighted in red.

6. Use the arrow keys and scroll wheel or number pad to enter the Clear From address.



7. Press F2 (Enter) to save the settings.

8. Press Return to return to the previous menu.

9. Repeat steps 4~8 for Length (F2).

10. Press F3 (Done) to clear the selected section of the arbitrary waveform.

Delete All

11. Press F4 (ALL) to delete the whole waveform.

12. Press F1 (Done) again to confirm the deletion.

13. Press Return return to the previous menu.



Clear From: 20, Length: 33.

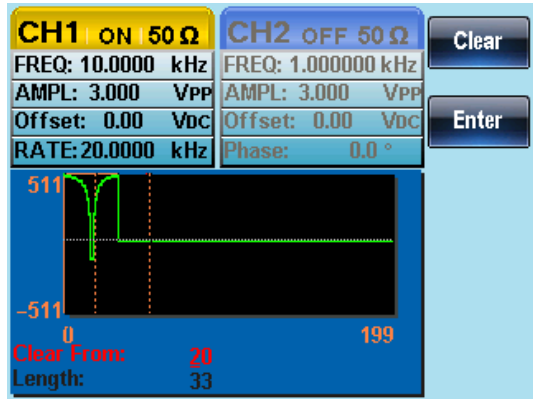

The same area after being cleared:

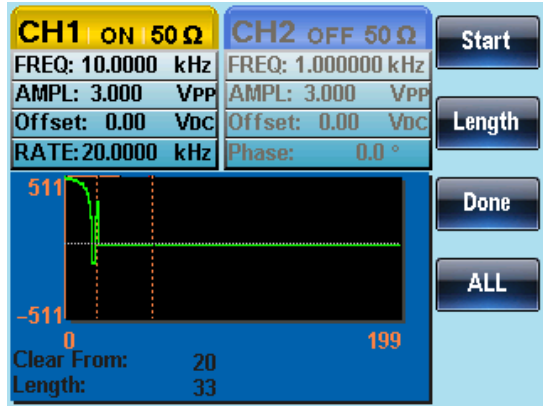

The result after the whole waveform is deleted:

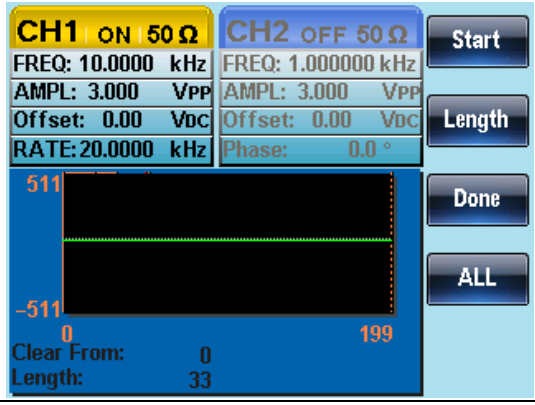

ARB Protection

The protection function designates an area of the arbitrary waveform that cannot be altered.

Panel Operation

1. Press the ARB key.

2. Press F2 (Edit).

3. Press F5 (Protect).

4. Press F2 (Start).

5. The Protect Start properties will become highlighted in red.

6. Use the arrow keys and scroll wheel or number pad to enter the Protect Start address.



7. Press F2 (Enter) to save the settings.

8. Press Return to return to the previous menu.



9. Repeat steps 4~8 for Length (F3).

10. Press F4 (Done) to confirm the protected area.

Protect All

11. Press F1 (ALL) to protect the whole waveform.

12. Press F1 (Done) to confirm.

Unprotect All

13. Press F5 (Unprotect) to unprotect the whole waveform.

14. Press F1 (Done) to confirm.

15. The waveform background will return back to black. The property “Protect Off” be will grayed out.

Below, the protected areas of the waveform are shown with an orange background:

Start:0, Length: 100.

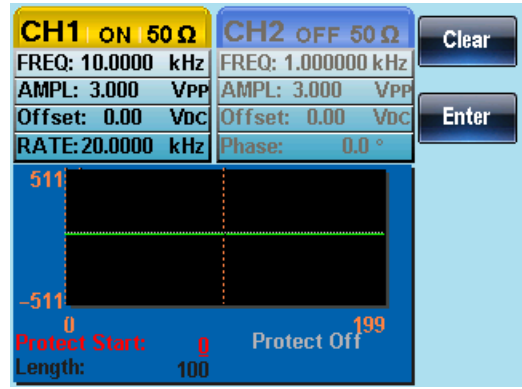

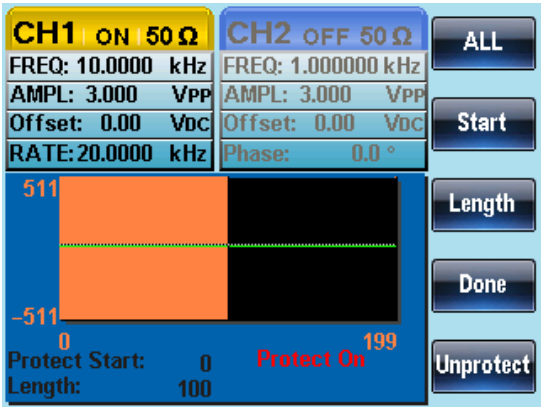

Ouput an Arbitrary Waveform

The arbitrary waveform generator can output up to 4k points (2~4096).

Ouput Arbitrary Waveform

Panel Operation

1. Press the ARB key.

2. Press F4 (Output).

3. Press F1 (Start).

4. The Start property will become highlighted in red.

5. Use the arrow keys and scroll wheel or number pad to enter the Start address.



6. Press F2 (Enter) to confirm the start point.

7. Press Return to return to the previous menu.



8. Repeat steps 4~7 for Length (F2).

9. Press Return to return to the previous menu.



The front panel terminal will output the following waveform.

Start 0，Length 500

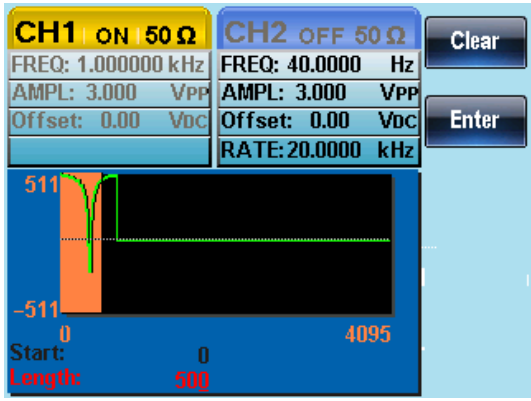

*ARB Marker Output

When turning on the ARB functionality,whether the ARB waveform is being output or not,there is a pulse from the Trigger OUT port. The pulse time is 1/RATE

Saving/Loading an Arbitrary Waveform

The AFG-2225 can save and load arbitrary waveforms from 10 internal memory slots. Arbitrary waveforms can also be saved and loaded from a USB memory stick.

Saving a Waveform to Internal Memory

Panel Operation

1. Press the ARB key.

2. Press F5 (More).

3. Press F1 (Save).

4. Press F1 (Start).

5. The Start property will become highlighted in red.

6. Use the arrow keys and scroll wheel or number pad to enter the Start address.



7. Press F2 (Enter) to confirm the start point.

8. Press Return to return to the previous menu.



9. Repeat steps 4~8 for Length (F2).

10. Press F3 (Memory).

11. Select a memory file using the scroll wheel.



Memory0~Memory9

12. Press F1 (Select) to save the selected memory file.

13. Press Return to return to the previous menu.

Below the file Memory0 is selected using the scroll wheel.

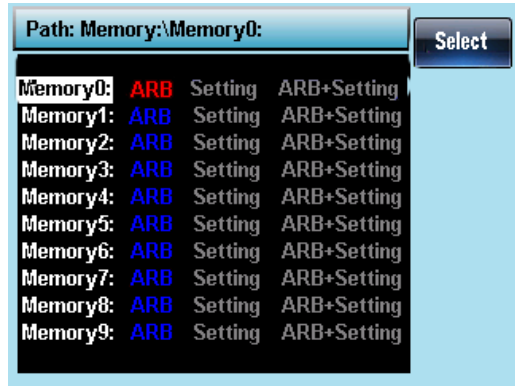

Saving a Waveform to USB Memory

Panel Operation

1. Press the ARB key.

2. Press F5 (More).

3. Press F1 (Save).

4. Press F1 (Start).

5. The Start propery will become highlighted in red.

6. Use the arrow keys and scroll wheel or number pad to enter the Start address.



7. Press F2 (Enter) to confirm the start point.

8. Press Return to return to the previous menu.

9. Repeat steps 4~8 for Length (F2).

10. Press F4 (USB).

11. Use the scroll wheel to navigate the file system.



12. Press Select to select directories or files.

Create a Folder

1. Press F2 (New Folder).

2. The text editor will appear with a default folder name of “NEW_FOL”.

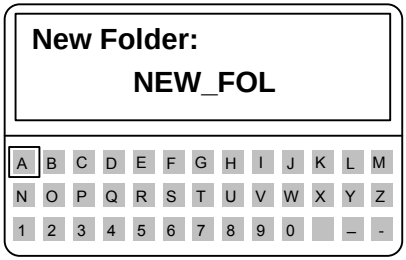

3. Use the scroll wheel to move the cursor.



4. Use F1 (Enter Char) or F2 (Backspace) to create a folder name.



5. Press F5 (Save) to save the folder name.

Create a New File

1. Press F3 (New File).

2. The text editor will appear with a default file name of "NEW_FIL".

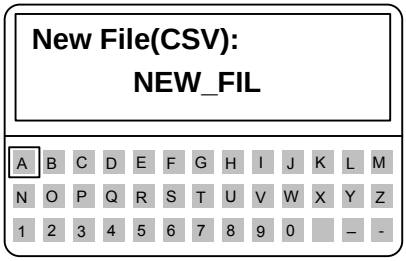

3. Use the scroll wheel to move the cursor.



4. Use F1 (Enter Char) or F2 (Backspace) to create a file name.



5. Press F5 (Save) to save the file name.

Below the folder, BIN, has been created in the root directory.

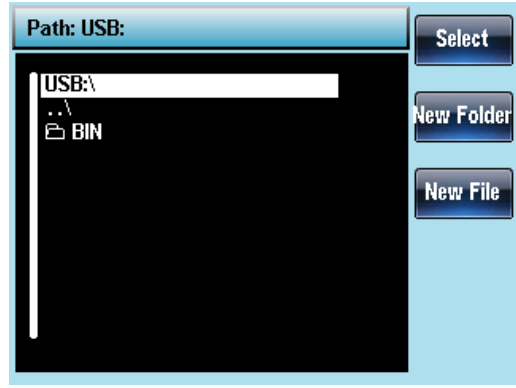

Load a Waveform from Internal Memory

Panel Operation

1. Press the ARBkey.

2. Press F5 (More).

3. Press F2 (Load).

4. Press F1 (Memory).

5. Use the scroll whell to choose a memory file.



6. Press Select to load the selected memory file.

7. Press F3 (To) to choose the starting point for the loaded waveform.

8. The Load To parameter will become highlighted in red.

9. Use the selector keys and scroll wheel or number pad to enter the starting point.



10. Press F2(Enter) to confirm the start point.

11. Press Return to return to the previous menu.

12. Press F4(Done).

Below the file Memory0 is selected using the scroll wheel loaded to position 0.

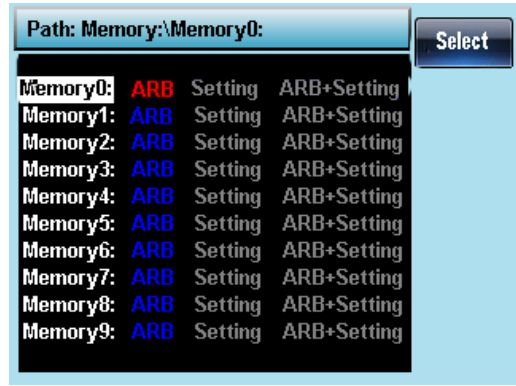
Path: Memory:\Memory0:
Select
Memory0: ARB Setting ARB+Setting
Memory1: ARB Setting ARB+Setting
Memory2: ARB Setting ARB+Setting
Memory3: ARB Setting ARB+Setting
Memory4: ARB Setting ARB+Setting
Memory5: ARB Setting ARB+Setting
Memory6: ARB Setting ARB+Setting
Memory7: ARB Setting ARB+Setting
Memory8: ARB Setting ARB+Setting
Memory9: ARB Setting ARB+Setting

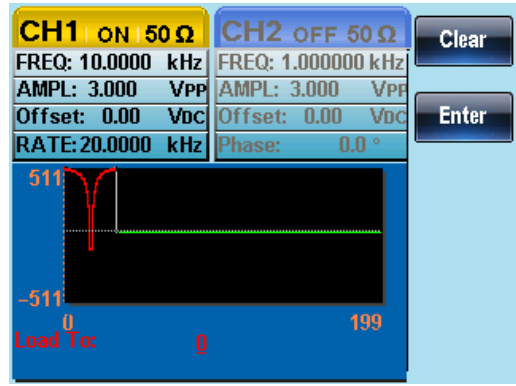
CH1 ON 50 Ω
FREQ: 10.0000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
RATE: 20.0000 kHz
CH2 OFF 50 Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Phase: 0.0 °
Clear
Enter
511
-511
0
199
Load To: 0

Load a Waveform from USB

Panel Operation

1. Press the ARB key.

2. Press F5 (More).

3. Press F2 (Load).

4. Press F2 (USB).

5. Use the scroll wheel to choose a file name.



6. Press F1 (Select) to select the file to load.

7. Press F3 (To) to choose the starting point for the loaded waveform.

8. The Load To property will become highlighted in red.

9. Use the arrow keys and scroll wheel or number pad to enter the starting point.



10. Press F2(Enter) to confirm the Start point.

11. Press F4(Done).

Below the file AFG.CSV is selected using the scroll wheel loaded to position 0.

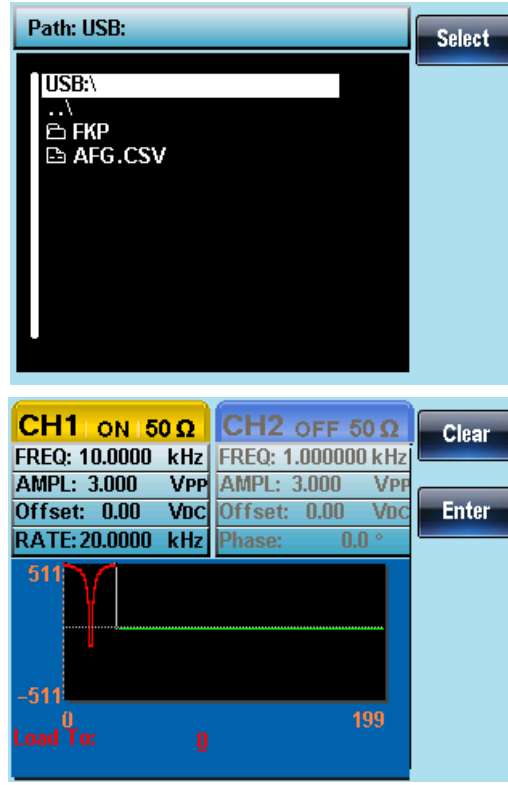

REMOTE INTERFACE

Establishing a Remote Connection 181
Configure USB interface 181
Remote control terminal connection 182
Command Syntax 184

Establishing a Remote Connection

The AFG-2225 supports USB remote connections.

Configure USB interface

USB configuration	PC side connector	Type A, host
	AFG-2225 side connector	Type B, slave
	Speed	1.1/2.0 (full speed)

Panel Operation

1. Connect the USB cable to the rear panel USB B (slave) port.

2. When the PC asks for the USB driver, select XXXXXXX.inf included in the software package or download the driver from the GW website, www.gwinstek.com.

Remote control terminal connection

Terminal application	Invoke the terminal application such as MTTTY (Multi-Threaded TTY). For USB, set the COM port, baud rate, stop bit, data bit, and parity accordingly. To check the COM port No, see the Device Manager in the PC. For WinXP, Control panel → System → Hardware tab.
Functionality check	Run this query command via the terminal. *idn? This should return the Manufacturer, Model number, Serial number, and Firmware version in the following format. GW INSTEK, AFG-2225, SN:XXXXXXXX,Vm.mm Note: ^j or ^m can be used as the terminal character when using a terminal program.
PC Software	The proprietary PC software, downloadable from GWInstek website, can be used for remote control.
Display	When a remote connection is established all panel keys are locked bar F5. 1. Press REM/LOCK (F5) to return the function generator to local mode.

CH1 ON 50Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Phase: 0.0 °
Ampl
DC Offset
1/FREQ
CH2 OFF 50Ω
FREQ: 1.000000 kHz
AMPL: 3.000 VPP
Offset: 0.00 VDC
Phase: 0.0 °
Ampl
DC Offset
1/FREQ
REM/LOC

Command Syntax

Compatible standard	• IEEE488.2, 1992 (fully compatible) • SCPI, 1994 (partially compatible)

Command Tree

The SCPI standard is an ASCII based standard that defines the command syntax and structure for programmable instruments.

Commands are based on a hierarchical tree structure. Each command keyword is a node on the command tree with the first keyword as the root node. Each sub node is separated with a colon.

Shown below is a section of the SOURce[1|2] root node and the :PM and :PULSe sub nodes.

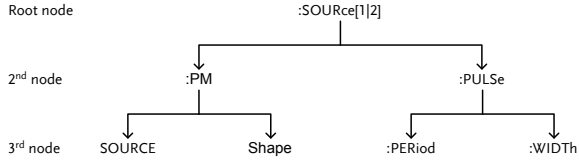

Command types

Commands can be separated in to three distinc types, simple commands, compound commands and queries.

Simple	A single command with/without a parameter
Example	*OPC
Compound	Two or more commands separated by a colon (:) with/without a parameter
Example	SOURce1:PULSe:WIDTh

	Query	A query is a simple or compound command followed by a question mark (?). A parameter (data) is returned. The maximum or minimum value for a parameter can also be queried where applicable.
	Example	SOURce1:FREQuency? SOURce1:FREQuency? MIN

Command forms

Commands and queries have two different forms, long and short. The command syntax is written with the short form of the command in capitals and the remainder (long form) in lower case.



The commands can be written in capitals or lower-case, just so long as the short or long forms are complete. An incomplete command will not be recognized.

Below are examples of correctly written commands:

LONG	SOURce1:DCOffset
	SOURCE1:DCOFFSET
	source1:dcoffset
SHORT	SOUR1:DCO
	sour1:dco

Command Format		1: command header 2: single space 3: parameter 4: message terminator
Square Brackets []	Commands that contain squares brackets indicate that the contents are optional. The function of the command is the same with or without the square bracketed items. Brackets are not sent with the command. For example, the frequency query below can use any of the following 3 forms: SOURce1:FREQuency? [MINimum|MAXimum] SOURce1:FREQuency? MAXimum SOURce1:FREQuency? MINimum SOURce1:FREQuency?	
Braces {}	Commands that contain braces indicate one item within the braces must be chosen. Braces are not sent with the command.	
Angled Brackets <>	Angle brackets are used to indicate that a value must be specified for the parameter. See the parameter description below for details. Angled brackets are not sent with the command.	
Bars |	Bars are used to separate multiple parameter choices in the command format.	

Parameters

Type	Description	Example
<Boolean>	Boolean logic	0, 1/ON,OFF
<NR1>	integers	0, 1, 2, 3
<NR2>	decimal numbers	0.1, 3.14, 8.5
<NR3>	floating point	4.5e-1, 8.25e+1
<NRf>	any of NR1, 2, 3	1, 1.5, 4.5e-1

	<NRf+> <Numeric>	NRf type with a suffix including MINimum, MAXimum or DEFault parameters.	1, 1.5, 4.5e-1 MAX, MIN,
	<aard>	Arbitrary ASCII characters.	
	<discrete>	Discrete ASCII character parameters	IMM, EXT, MAN
	<frequency> <peak deviation in Hz> <rate in Hz>	NRf+ type including frequency unit suffixes.	1 KHZ, 1.0 HZ, MHZ
	<amplitude>	NRf+ type including voltage peak to peak.	VPP
	<offset>	NRf+ type including volt unit suffixes.	V
	<seconds>	NRf+ type including time unit suffixes.	NS, S MS US
	<percent> <depth in percent>	NRf type	N/A
Message terminators	LF CR	line feed code (new line) and carriage return.	
	LF	line feed code (new line)	
	EOI	IEEE-488 *EOI* (End-Or-Identify)	
Note	∧j or ∧m should be used when using a terminal program.		

Command Separators	Space	A space is used to separate a parameter from a keyword/command header.
	Colon (:)	A colon is used to separate keywords on each node.
	Semicolon (;)	A semi colon is used to separate subcommands that have the same node level. For example: SOURce[1|2]:DCOffset? SOURce[1|2]:OUTPut? →SOURce1:DCOffset?;OUTPut?
	Colon + Semicolon (:;)	A colon and semicolon can be used to combine commands from different node levels. For example: SOURce1:PM:SOURce? SOURce:PULSe:WIDTh? →SOURce1:PM:SOURce?:;SOURce:PULSe:WIDTh?
	Comma (,)	When a command uses multiple parameters, a comma is used to separate the parameters. For example: SOURce:APPLy:SQUare 10KHZ, 2.0 VPP, -1V

Command List

System Commands 193
SYSTem:ERRor? 193
*IDN? 193
*RST 194
SYSTem:VERSion? 194
*OPC 194
*OPC? 195
*WAI 195
Status Register Commands 196
*CLS 196
*ESE 196
*ESR? 197
*STB? 197
*SRE 198
System Remote Commands 199
SYSTem:LOCal 199
SYSTem:REMote 199
DISPlay ON/OFF 199
Apply Commands 200
SOURce[1|2]:APPLy:SINusoid 202
SOURce[1|2]:APPLy:SQUare 202
SOURce[1|2]:APPLy:RAMP 203
SOURce[1|2]:APPLy:PULSe 203
SOURce[1|2]:APPLy:NOISe 204
SOURce[1|2]:APPLy:USER 204
SOURce[1|2]:APPLy? 205
Output Commands 206
SOURce[1|2]:FUNCtion 206
SOURce[1|2]:FREQuency 207
SOURce[1|2]:AMPlitude 209
SOURce[1|2]:DCOffset 210
SOURce[1|2]:SQUare:DCYCle 211
SOURce[1|2]:RAMP:SYMMetry 212
OUTPut[1|2] 213
OUTPut[1|2]:LOAD 213
SOURce[1|2]:VOLTage:UNIT 214
Pulse Configuration Commands 216
SOURce[1|2]:PULSe:PERiod 216
SOURce[1|2]:PULSe:WIDTh 217
Amplitude Modulation (AM) Commands 218
AM Overview 218

SOURce[1|2]:AM:STATe 219
SOURce[1|2]:AM:SOURce 219
SOURce[1|2]:AM:INTernal:FUNCtion 220
SOURce[1|2]:AM:INTernal:FREQuency 221
SOURce[1|2]:AM:DEPTh 221
Frequency Modulation (FM) Commands 223
FM Overview 223
SOURce[1|2]:FM:STATe 224
SOURce[1|2]:FM:SOURce 224
SOURce[1|2]:FM:INTernal:FUNCtion 225
SOURce[1|2]:FM:INTernal:FREQuency 226
SOURce[1|2]:FM:DEViation 226
Frequency-Shift Keying (FSK) Commands 228
FSK Overview 228
SOURce[1|2]:FSKey:STATe 228
SOURce[1|2]:FSKey:SOURce 229
SOURce[1|2]:FSKey:FREQuency 229
SOURce[1|2]:FSKey:INTernal:RATE 230
Phase Modulation (PM)Commands 232
PM Overview 232
SOURce[1|2]:PM:STATe 233
SOURce[1|2]:PM:SOURce 233
SOURce[1|2]:PM:INTernal:FUNction 234
SOURce[1|2]:PM:INTernal:FREQuency 234
SOURce[1|2]:PM:DEViation 235
SUM Modulation (SUM) Commands 236
SUM Overview 236
SOURce[1|2]:SUM:STATe 237
SOURce[1|2]:SUM:SOURce 237
SOURce[1|2]:SUM:INTernal:FUNction 238
SOURce[1|2]:SUM:INTernal:FREQuency 238
SOURce[1|2]:SUM:AMPL 239
Frequency Sweep Commands 240
Sweep Overview 240
SOURce[1|2]:SWEep:STATe 241
SOURce[1|2]:FREQuency:STARt 242
SOURce[1|2]:FREQuency:STOP 242
SOURce[1|2]:FREQuency:CENTer 243
SOURce[1|2]:FREQuency:SPAN 244
SOURce[1|2]:SWEep:SPACing 245
SOURce[1|2]:SWEep:TIME 245
SOURce[1|2]:SWEep:SOURce 246
SOURce[1|2]:MARKer:FREQuency 247
SOURce[1|2]:MARKer 247

Burst Mode Commands 249
Burst Mode Overview 249
SOURce[1|2]:BURSt:STATe 251
SOURce[1|2]:BURSt:MODE 251
SOURce[1|2]:BURSt:NCYCles 252
SOURce[1|2]:BURSt:INTernal:PERiod 253
SOURce[1|2]:BURSt:PHASe 254
SOURce[1|2]:BURSt:TRIGger:SOURce 254
SOURce[1|2]:BURSt:TRIGger:DELay 255
SOURce[1|2]:BURSt:TRIGger:SLOPe 256
SOURce[1|2]:BURSt:TRIGger:MANual 257
SOURce[1|2]:BURSt:GATE:POLarity 257
SOURce[1|2]:BURSt:OUTPut:TRIGger:SLOPe 258
OUTPut[1|2]:TRIGger 259
Arbitrary Waveform Commands 260
Arbitrary Waveform Overview 260
SOURce[1|2]:FUNCtion USER 261
SOURce[1|2]:DATA:DAC 261
SOURce[1|2]:ARB:EDIT:COPY 262
SOURce[1|2]:ARB:EDIT:DELete 263
SOURce[1|2]:ARB:EDIT:DELete:ALL 263
SOURce[1|2]:ARB:EDIT:POINt 263
SOURce[1|2]:ARB:EDIT:LINE 264
SOURce[1|2]:ARB:EDIT:PROTect 264
SOURce[1|2]:ARB:EDIT:PROTect:ALL 265
SOURce[1|2]:ARB:EDIT:UNProtect 265
SOURce[1|2]:ARB:OUTPut 265
COUNTER 266
COUNTER:STATE 266
COUNter:GATe 266
COUNter:VALue? 267
PHASE 267
SOURce[1|2]:PHASe 267
SOURce[1|2]:PHASe:SYNChronize 268
SOURce[1|2]:PHASe:SYNChronize 268
SOURce1:PHASe:SYNChronize 268
COUPLE 268
SOURce[1|2]:FREQuency:COUPle:MODE 268
SOURce[1|2]:FREQuency:COUPle:OFFSet 269
SOURce[1|2]:FREQuency:COUPle:RATio 269
SOURce[1|2]:AMPlitude:COUPle:STATe 269
SOURce[1|2]:TRACk 270
Save and Recall Commands 271
*SAV 271

*RCL 271
MEMory:STATe:DELete 271
MEMory:STATe:DELete ALL 272

System Commands

SYSTem:ERRor? System Query

Description	Reads an error from the error queue. See page 286 for details regarding the error queue.	
Query Syntax	**SYSTem:ERRor?**	
Return parameter	<string>	Returns an error string, <256 ASCII characters.
Example	**SYSTem:ERRor?** **-138 Suffix not allowed** Returns an error string.	

*IDN? System Query

Description	Returns the function generator manufacturer, model number, serial number and firmware version number in the following format: GW INSTEK,AFG-2225,SN:XXXXXXXX,Vm.mm	
Query Syntax	***IDN?**	
Return parameter	<string>	
Example	***IDN?** GW INSTEK,AFG-2225,SN:XXXXXXXX,Vm.mm Returns the identification of the function generator.	

*RST System Command

Description	Reset the function generator to its factory default state.
Note	Note the *RST command will not delete instrument save states in memory.
Syntax	***RST**

SYSTem:VERSion? System Query

Description	Performs a system version query. Returns a string with the instrument, firmware version, FPGA revision
Query Syntax	**SYSTem:VERSion?**
Return parameter	<string>
Example	**SYST:VERS?** AFG-2225 VX.XXX_XXXX Returns the year and version for that year (1).

*OPC System Command

Description	This command sets the Operation Complete Bit (bit 0) of the Standard Event Status Register after the function generator has completed all pending operations. For the AFG-2225, the *OPC command is used to indicate when a sweep or burst has completed.
Note	Before the OPC bit is set, other commands may be executed.
Syntax	***OPC**

*OPC? System Query

Description	Returns the OPC bit to the output buffer when all pending operations have completed. I.e. when the OPC bit is set.
Note	Commands cannot be executed until the *OPC? query has completed.
Query Syntax	***OPC?**
Return parameter	1
Example	***OPC?** **1** Returns a "1" when all pending operations are complete.

*WAI System Command

Description	This command waits until all pending operations have completed before executing additional commands. I.e., when the OPC bit is set.
Note	This command is only used for triggered sweep and burst modes.
Syntax	***WAI**

Status Register Commands

*CLS

System Command

Description	The *CLS command clears all the event registers, the error queue and cancels an *OPC command.
Syntax	***CLS**

*ESE

System Command

Description	The Standard Event Status Enable command determines which events in the Standard Event Status Event register can set the Event Summary Bit (ESB) of the Status Byte register. Any bit positions set to 1 enable the corresponding event. Any enabled events set bit 5 (ESB) of the Status Byte register.
Note	The *CLS command clears the event register, but not the enable register.
Syntax	***ESE <enable value>**
Parameter	<enable value> 0~255
Example	***ESE 20** Sets a bit weight of 20 (bits 2 and 4).
Query Syntax	***ESE?**

Return Parameter

Bit	Register	Bit	Register
0	Not used	4	Message Available
1	Not used	5	Standard Event
2	Error Queue	6	Master Summary
3	Questionable Data	7	Not used

Example	***ESE?** **4** Bit 2 is set.

*ESR? System Command

Description	Reads and clears the Standard Event Status Register. The bit weight of the standard event status register is returned.
Note	The *CLS will also clear the standard event status register.
Query Syntax	***ESR?**

Return Parameter

Bit	Register	Bit	Register
0	Operation Complete	4	Execution Error
1	Not Used	5	Command Error
2	Query Error	6	Not Used
3	Device Error	7	Power On

Query Example	***ESR?** **5** Returns the bit weight of the standard event status register (bit 0 and 2).

*STB? System Command

Description	Reads the Status byte condition register.
Note	Bit 6, the master summary bit, is not cleared.
Syntax	***STB?**

*SRE System Command

Description	The Service Request Enable Command determines which events in the Status Byte Register are allowed to set the MSS (Master summary bit). Any bit that is set to "1" can cause the MSS bit to be set.			
Note	The *CLS command clears the status byte event register, but not the enable register.			
Syntax	***SRE <enable value>**			
Parameter	<enable value>	0~255		
Example	***SRE 12** Sets a bit weight of 12 (bits 2 and 3) for the service request enable register.			
Query Syntax	***SRE?**			
Return Parameter	Bit	Register	Bit	Register
	0	Not used	4	Message Available
	1	Not used	5	Standard Event
	2	Error Queue	6	Master Summary
	3	Questionable Data	7	Not used
Query Example	***SRE?** **12** Returns the bit weight of the status byte enable register.			

System Remote Commands

SYSTem:LOCal System Command

Description	Sets the function generator to local mode. In local mode, all front panel keys are operational.
Syntax	**SYSTem:LOCal**
Example	**SYST:LOC**

SYSTem:REMote System Command

Description	Disables the front panel keys and puts the function generator into remote mode
Syntax	**SYSTem:REMote**
Example	**SYST:REM**

DISPlay ON/OFF System Command

Description	Enable or disable the front panel display of function generator. When disabled, display does not display any content. Due to disabling the front panel display, the speed of executing commands from the remote interface will be improved.
Syntax	**DISPlay ON/OFF**
Example	**DISPlay ON**

Apply Commands

The APPLy command has 5 different types of outputs (Sine, Square, Ramp, Pulse, Noise,). The command is the quickest, easiest way to output waveforms remotely. Frequency, amplitude and offset can be specified for each function.

As only basic parameters can be set with the Apply command, other parameters use the instrument default values.

The Apply command will set the trigger source to immediate and disable burst, modulation and sweep modes. Turns on the output commandOUTPut[1|2] ON. The termination setting will not be changed.

As the frequency, amplitude and offset parameters are in nested square brackets, amplitude can only be specified if the frequency has been specified and offset can only be specified if amplitude has been set. For the example:

SOURce[1|2]:APPLy:SINusoid [<frequency> [,<amplitude> [,<offset>]]]

Output Frequency For the output frequency, MINimum, MAXimum and DEFault can be used. The default frequency for all functions is set to 1 kHz. The maximum and minimum frequency depends on the function used. If a frequency output that is out of range is specified, the max/min frequency will be used instead. A "Data out range error will be generated" from the remote terminal.

Output Amplitude	When setting the amplitude, MINimum, MAXimum and DEFault can be used. The range depends on the function being used and the output termination (50Ω or high impedance). The default amplitude for all functions is 100 mVpp (50Ω). If the amplitude has been set and the output termination is changed from 50Ω to high impedance, the amplitude will double. Changing the output termination from high impedance to 50Ω will half the amplitude. Vrms, dBm or Vpp units can be used to specify the output unit to use with the current command. The VOLT:UNIT command can be used to set the units when no unit is specified with the Apply command. If the output termination is set to high impedance, dBm units cannot be used. The units will default to Vpp. The output amplitude can be affected by the function and unit chosen. Vpp and Vrms or dBm values may have different maximum values due to differences such as crest factor. For example, a 5Vrms square wave must be adjusted to 3.536 Vrms for a sine wave.
DC Offset voltage	The offset parameter can be set to MINimum, MAXimum or DEFault. The default offset is 0 volts. The offset is limited by the output amplitude as shown below. $\|V_{offset}\| < V_{max} - Vpp/2$ If the output specified is out of range, the maximum offset will be set.

The offset is also determined by the output termination (50Ω or high impedance). If the offset has been set and the output termination has changed from 50Ω to high impedance, the offset will double. Changing the output termination from high impedance to 50Ω will half the offset.

SOURce[1|2]:APPLy:SINusoid

Source Specific Command

Description	Outputs a sine wave from the selected channel when the command has executed. Frequency, amplitude and offset can also be set.	
Syntax	SOURce[1|2]:APPLy:SINusoid [<frequency> [,<amplitude> [,<offset>]]]	
Parameter	<frequency>	1μHz~25MHz
	<amplitude>	1mVpp~10Vpp (50Ω) (3.536 Vrms)
	<offset>	-4.99V~4.99V (50Ω)
Example	**SOUR1:APPL:SIN 2KHZ,MAX,MAX** Sets frequency to 2kHz and sets the amplitude and offset to the maximum.	

SOURce[1|2]:APPLy:SQUare

Source Specific Command

Description	Outputs a square wave from the selected channel when the command has executed. Frequency, amplitude and offset can also be set. The duty cycle is set to 50%.	
Syntax	SOURce[1|2]:APPLy:SQUare [<frequency> [,<amplitude> [,<offset>]]]	
Parameter	<frequency>	1μHz~25MHz
	<amplitude>	1mVpp~10Vpp (50Ω)
	<offset>	-4.99V~4.99V (50Ω)
Example	**SOUR1:APPL:SQU 2KHZ,MAX,MAX**	

Sets frequency to 2kHz and sets the amplitude and offset to the maximum.

SOURce[1|2]:APPLy:RAMP

Source Specific Command

Description	Outputs a ramp wave from the selected channel when the command has executed. Frequency, amplitude and offset can also be set. The symmetry is set to 50%.	
Syntax	**SOURce[1|2]:APPLy:RAMP [<frequency> [,<amplitude> [,<offset>]]]**	
Parameter	<frequency>	1µHz~1MHz
	<amplitude>	1mVpp~10Vpp (50Ω)
	<offset>	-4.99V~4.99V (50Ω)
Example	**SOUR1:APPL:RAMP 2KHZ,MAX,MAX**	
	Sets frequency to 2kHz and sets the amplitude and offset to the maximum.	

SOURce[1|2]:APPLy:PULSe

Source Specific Command

Description	Outputs a pulse waveform from the selected channel when the command has executed. Frequency, amplitude and offset can also be set.	
Note	The PW settings from the SOURce[1|2]:PULS:WIDT command are preserved. Edge and pulse width may be adjusted to supported levels.	
	Repetition rates will be approximated from the frequency. For accurate repetition rates, the period should be adjusted using the SOURce[1|2]:PULS:PER command	
Syntax	**SOUR[1|2]:APPLy:PULSe [<frequency> [,<amplitude> [,<offset>]]]**	
Parameter	<frequency>	500µHz~25MHz
	<amplitude>	1mVpp~10Vpp (50Ω)

	<offset>	-4.99V~4.99V (50Ω)
Example	SOUR1:APPL:PULS 1KHZ,MIN,MAX Sets frequency to 1kHz and sets the amplitude to minimum and the and offset to the maximum.	

SOURce[1|2]:APPLy:NOISe

Source Specific Command

Description	Outputs Gaussian noise. Amplitude and offset can also be set.	
Note	Frequency cannot be used with the noise function; however a value (or DEFault) must be specified. The frequency is remembered for the next function used.	
Syntax	SOURce[1|2]:APPLy:NOISe [<frequency|DEFault> [,<amplitude> [,<offset>]]]	
Parameter	<frequency>	Not applicable
	<amplitude>	1mVpp~10Vpp (50Ω)
	<offset>	-4.99V~4.99V (50Ω)
Example	SOUR1:APPL:NOIS DEF, 3.0, 1.0 Sets the amplitude to 3 volts with an offset of 1 volt.	

SOURce[1|2]:APPLy:USER

Source Specific Command

Description	Outputs an arbitrary waveform from the selected channel. The output is that specified from the FUNC:USER command.
Note	Frequency and amplitude cannot be used with the DC function; however a value (or DEFault) must be specified. The values are remembered for the next function used.

Syntax	**SOURce[1|2]:APPLy:USER [<frequency> [,<amplitude> [,<offset>]]]**	
Parameter	<frequency>	1µHz~60MHz
	<amplitude>	1mVpp~10Vpp (50Ω)
	<offset>	-4.99V~4.99V (50Ω)
Example	**SOUR1:APPL:USER**	

SOURce[1|2]:APPLy?

Source Specific Command

Description	Outputs a string with the current settings.	
Note	The string can be passed back appended to the Apply Command.	
Syntax	**SOURce[1|2]:APPLy?**	
Return Parameter	<string>	Function, frequency, amplitude, offset
Example	**SOUR1:APPL?** SIN +5.0000000000000E+03,+3.0000E+00,-2.50E+00 Returns a string with the current function and parameters, Sine, 5kHz, 3 Vpp, -2.5V offset.	

Output Commands

Unlike the Apply commands, the Output commands are low level commands to program the function generator.

This section describes the low-level commands used to program the function generator. Although the APPLy command provides the most straightforward method to program the function generator, the low-level commands give you more flexibility to change individual parameters.

SOURce[1|2]:FUNCtion

Source Specific Command

Description	The FUNCtion command selects and outputs the selected output. The User parameter outputs an arbitrary waveform previously set by the SOURce[1|2]:FUNC:USER command.
Note	If the function mode is changed and the current frequency setting is not supported by the new mode, the frequency setting will be altered to next highest value. Vpp and Vrms or dBm amplitude values may have different maximum values due to differences such as crest factor. For example, if a 5Vrms square wave is changed to a sinewave, then the Vrms is automatically adjusted to 3.536. The modulation, burst and sweep modes can only be used with some of the basic waveforms. If a mode is not supported, the conflicting mode will be disabled. See the table below.

	Sine	Square	Ramp	Pulse	Noise	ARB
AM	✓	✓	✓	✓	×	✓
FM	✓	✓	✓	×	×	×
PM	✓	✓	✓	×	×	×
FSK	✓	✓	✓	✓	×	×
SUM	✓	✓	✓	✓	✓	×
SWEEP	✓	✓	✓	×	×	×
BURST	✓	✓	✓	×	×	×

Syntax	**SOURce[1|2]:FUNCtion {SINusoid|SQUare|RAMP| PULSe|NOISe| USER}**
Example	**SOUR1:FUNC SIN** Sets the output as a sine function.
Query Syntax	**SOURce[1|2]:FUNCtion?**
Return Parameter	SIN, SQU, RAMP, PULS, NOIS, USER — Returns the current output type.
Example	**SOUR1:FUNC?** SIN Current output is sine.

SOURce[1|2]:FREQuency

Source Specific Command

Description	The SOURce[1|2]:FREQuency command sets the output freuquency for the selected channel. The query command returns the current frequency setting.
Note	The maximum and minimum frequency depends on the function mode.

Sine, Square	1μHz~25MHz
Ramp	1μHz~1MHz
Pulse	500μHz~25MHz

	Noise	Not applicable
	User	1μHz~60MHz

If the function mode is changed and the current frequency setting is not supported by the new mode, the frequency setting will be altered to next highest value.

The duty cycle of square waveforms depends on the frequency settings.

1.0% to 99.0%(*frequency*≤100 KHz)

10% to 90% (100 KHz ≤ *frequency* ≤1MHz)

50% (*frequency* ≤ 25 MHz)

If the frequency is changed and the set duty cycle cannot support the new frequency, the highest duty cycle available at that frequency will be used. A "settings conflict" error will result from the above scenario.

Syntax	**SOURce[1|2]:FREQuency {<frequency>|MINimum|MAXimum}**
Example	**SOUR1:FREQ MAX** Sets the frequency to the maximum for the current mode.
Query Syntax	**SOURce[1|2]:FREQuency?**

Return Parameter	<NR3>	Returns the frequency for the current mode.

Example	**SOUR1:FREQ? MAX** +1.0000000000000E+06 The maximum frequency that can be set for the current function is 1MHz.

SOURce[1|2]:AMPlitude

Source Specific Command

Description

The SOURce[1|2]:AMPLitude command sets the output amplitude for the selected channel. The query command returns the current amplitude settings.

Note

The maximum and minimum amplitude depends on the output termination. The default amplitude for all functions is 100 mVpp (50Ω). If the amplitude has been set and the output termination is changed from 50Ω to high impedance, the amplitude will double. Changing the output termination from high impedance to 50Ω will half the amplitude.

The offset and amplitude are related by the following equation.
$|V_{offset}| < V_{max} - Vpp/2$

If the output termination is set to high impedance, dBm units cannot be used. The units will default to Vpp.

The output amplitude can be affected by the function and unit chosen. Vpp and Vrms or dBm values may have different maximum values due to differences such as crest factor. For example, a 5Vrms square wave must be adjusted to 3.536 Vrms for a sine wave.

The amplitude units can be explicitly used each time the SOURce[1|2]:AMPlitude command is used. Alternatively, the VOLT:UNIT command can be used to set the amplitude units for all commands.

Syntax	**SOURce[1|2]:AMPlitude {< amplitude> |MINimum|MAXimum}**	
Example	**SOUR1:AMP MAX** Sets the amplitude to the maximum for the current mode.	
Query Syntax	**SOURce[1|2]:AMPlitude? {MINimum|MAXimum}**	
Return Parameter	<NR3>	Returns the amplitude for the current mode.
Example	**SOUR1:AMP? MAX** +5.0000E+00 The maximum amplitude that can be set for the current function is 5 volts.	

SOURce[1|2]:DCOffset

Source Specific Command

Description	Sets or queries the DC offset for the current mode.
Note	The offset parameter can be set to MINimum, MAXimum or DEFault. The default offset is 0 volts. The offset is limited by the output amplitude as shown below. $\|V_{offset}\| < V_{max} - Vpp/2$ If the output specified is out of range, the maximum offset will be set. The offset is also determined by the output termination (50Ω or high impedance). If the offset has been set and the output termination has changed from 50Ω to high impedance, the offset will double. Changing the output termination from high impedance to 50Ω will half the offset.

Syntax	**SOURce[1|2]:DCOffset {< offset> |MINimum|MAXimum}**
Example	**SOUR1:DCO MAX** Sets the offset to the maximum for the current mode.
Query Syntax	**SOURce[1|2]:DCOffset? {MINimum|MAXimum}**
Return Parameter	<NR3> Returns the offset for the current mode.
Example	**SOUR1:DCO?** +3.0000E+00 The offset for the current mode is set to +3 volts.

SOURce[1|2]:SQUare:DCYCle

Source Specific Command

Description	Sets or queries the duty cycle for square waves only. The setting is remembered if the function mode is changed. The default duty cycle is 50%.
Note	The duty cycle of square waveforms depend on the frequency settings. 1.0% to 99.0%(*frequency*≤100 KHz) 10% to 90% (100 KHz ≤ *frequency* ≤1MHz) 50% (*frequency* ≤ 25 MHz) If the frequency is changed and the set duty cycle cannot support the new frequency, the highest duty cycle available at that frequency will be used. A "settings conflict" error will result from the above scenario. For square waveforms, the Apply command and AM/FM modulation modes ignore the duty cycle settings.
Syntax	**SOURce[1|2]:SQUare:DCYCle {< percent> |MINimum|MAXimum}**

Example	**SOUR1:SQU:DCYC MAX** Sets the duty cycle to the highest possible for the current frequency.	
Query Syntax	**SOURce[1|2]:SQUare:DCYCle? {MINimum|MAXimum}**	
Return Parameter	<NR3>	Returns the duty cycle as a percentage.
Example	**SOUR1:SQU:DCYC?** +5.00E+01 The duty cycle is set 50%.	

SOURce[1|2]:RAMP:SYMMetry

Source Specific Command

Description	Sets or queries the symmetry for ramp waves only. The setting is remembered if the function mode is changed. The default symmetry is 50%.	
Note	For ramp waveforms, the Apply command and AM/FM modulation modes ignore the current symmetry settings.	
Syntax	**SOURce[1|2]:RAMP:SYMMetry {< percent> |MINimum|MAXimum}**	
Example	**SOUR1:RAMP:SYMM MAX** Sets the symmetry to the 100%.	
Query Syntax	**SOURce[1|2]:RAMP:SYMMetry? {MINimum|MAXimum}**	
Return Parameter	<NR3>	Returns the symmetry as a percentage.
Example	**SOUR1:RAMP:SYMMetry?** +1.0000E+02 The symmetry is set as 100%.	

OUTPut[1|2]

Source Specific Command

Description	Enables/Disables or queries the front panel output from the selected channel. The default is set to off.
Note	If the output is overloaded by an external voltage, the output will turn off and an error message will be displayed. The overload must first be removed before the output can be turned on again with output command. Using the Apply command automatically sets the front panel output to on.
Syntax	**OUTPut[1|2] {OFF|ON}**
Example	**OUTP1 ON** Turns the channel 1 output on.
Query Syntax	**OUTPut[1|2]?**

Return Parameter		
	1	ON
	0	OFF

Example	**OUTP1?** **1** The channel 1 output is currently on.

OUTPut[1|2]:LOAD

Source Specific Command

Description	Sets or queries the output termination. Two impedance settings can be chosen, DEFault (50Ω) and INFinity (high impedance >10 kΩ). The output termination is to be used as a reference only. If the output termination is set 50Ω but the actual load impedance is not 50Ω, then the amplitude and offset will not be correct.
Note	If the amplitude has been set and the output termination is changed from 50Ω to high impedance, the amplitude will double. Changing

	the output termination from high impedance to 50Ω will half the amplitude. If the output termination is set to high impedance, dBm units cannot be used. The units will default to Vpp.	
Syntax	**OUTPut[1|2]:LOAD {DEFault|INFinity}**	
Example	**OUTP1:LOAD DEF** Sets the channel 1 output termination to 50Ω.	
Query Syntax	**OUTPut[1|2]:LOAD?**	
Return Parameter	DEF	Default
	INF	INFinity
Example	**OUTP1:LOAD?** **DEF** The output termination for channel 1 is set to 50Ω.	

SOURce[1|2]:VOLTage:UNIT

Source Specific Command

Description	Sets or queries the output amplitude units. There are three types of units: VPP, VRMS and DBM.	
Note	The units set with the VOLTage:UNIT command will be used as the default unit for all amplitude units unless a different unit is specifically used for a command. If the output termination is set to high impedance, dBm units cannot be used. The Units will automatically default to Vpp.	
Syntax	**SOURce[1|2]:VOLTage:UNIT {VPP|VRMS|DBM}**	
Example	**SOUR1:VOLT:UNIT VPP** Sets the amplitude units to Vpp.	
Query Syntax	**SOURce[1|2]:VOLTage:UNIT?**	
Return Parameter	VPP	Vpp
	VRMS	Vrms

	DBM	dBm

Example **SOUR1:VOLT:UNIT?**

VPP

The amplitude units are set to Vpp.

Pulse Configuration Commands

The pulse chapter is used to control and output pulse waveforms. Unlike the APPLy command, low level control is possible including setting the rise time, fall time, period and pulse width.

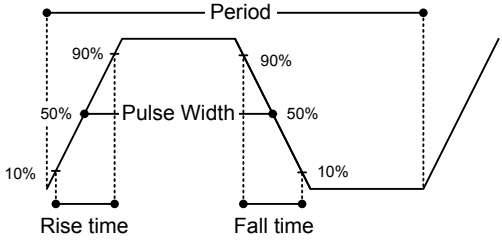

SOURce[1|2]:PULSe:PERiod

Source Specific Command

Description	Sets or queries the pulse period. The default period is 1 ms.
Note	The pulse period must be greater than the pulse width and edge time(1.6x) combined. Pulse Width + (1.6 * Edge Time) < Period If the edge time or pulse width are too great, they will automatically be reduced to fit the period by the function generator. The PULSe:PERiod function will change the period for all functions, not just for the pulse waveforms. If a different function is chosen and the current period is out of range, the period will be automatically adjusted to suit the new function.
Syntax	**SOURce[1|2]:PULSe:PERiod {<seconds>|MINimum|MAXimum}**
Example	**SOUR1:PULS:PER MIN** Sets the period to the minimum time allowed.
Query Syntax	**SOURce[1|2]:PULSe:PERiod? [MINimum|MAXimum]**
Return Parameter	<seconds> 40ns~2000s

Example	SOUR1:PULS:PER? +1.0000E+01 The period is set to 10 seconds.

SOURce[1|2]:PULSe:WIDTh

Source Specific Command

Description	Sets or queries the pulse width. The default pulse width is 100us. The minimum pulse width is affected by the period time. If the period is over 20 or 200 seconds, then the minimum pulse width is 1us and 10us, respectively. Pulse width is defined as the time from the rising to falling edges (at a threshold of 50%).
Note	The pulse width cannot be less than the edge time times 1.6. Pulse Width > 1.6 * Edge Time The pulse width must be less than the period minus the edge time (x1.6). Pulse Width < Period – (1.6 *Edge Time)
Syntax	SOURce[1|2]:PULSe:WIDTh {<seconds>|MINimum|MAXimum}
Example	SOUR1:PULS:WIDT MAX Sets the pulse width to the maximum allowed.
Query Syntax	SOURce[1|2]:PULSe:WIDTh? [MINimum|MAXimum]
Return Parameter	<seconds> 20 ns ~ 1999.9 seconds
Example	SOUR1:PULS:WIDT? MIN +8.0000E-09 The pulse width is set to 8 nanoseconds.

Amplitude Modulation (AM) Commands

AM Overview

To successfully create an AM waveform, the following commands must be executed in order.

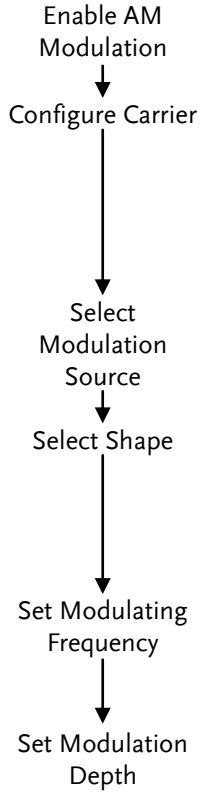

2. Turn on AM modulation using the SOURce[1|2]: AM:STAT ON command
3. Use the APPLy command to select a carrier waveform. Alternatively the equivalent FUNC, FREQ, AMPl, and DCOffs commands can be used to create a carrier waveform with a designated frequency, amplitude and offset.
4. Select an internal or external modulation source using the SOURce[1|2]:AM:SOUR command.
5. Use the SOURce[1|2]:AM:INT:FUNC command to select a sine, square, upramp, dnramp or triangle modulating waveshape. For internal sources only.
6. Set the modulating frequency using the SOURce[1|2]: AM:INT:FREQ command. For internal sources only.
7. Set the modulation depth using the SOURce[1|2]: AM:DEPT command.

SOURce[1|2]:AM:STATe

Source Specific Command

Description	Sets or disables AM modulation. By default AM modulation is disabled. AM modulation must be enabled before setting other parameters.	
Note	Burst or sweep mode will be disabled if AM modulation is enabled. As only one modulation is allowed at any one time, other modulation modes will be disabled when AM modulation is enabled.	
Syntax	**SOURce[1|2]:AM:STATe {OFF|ON}**	
Example	**SOUR1:AM:STAT ON** Enables AM modulation.	
Query Syntax	**SOURce[1|2]:AM:STATe?**	
Return Parameter	0	Disabled (OFF)
	1	Enabled (ON)
Example	**SOUR1:AM:STAT?** **1** AM modulation mode is currently enabled.	

SOURce[1|2]:AM:SOURce

Source Specific Command

Description	Sets or queries the modulation source as internal or external. Internal is the default modulation source.
Note	If an external modulation source is selected, modulation depth is limited to ± 5V from the MOD INPUT terminal on the rear panel. For example, if modulation depth is set to 100%, then the maximum amplitude is +5V, and the minimum amplitude is -5V.
Syntax	**SOURce[1|2]:AM:SOURce {INTernal|EXTernal}**

Example	**SOUR1:AM:SOUR EXT**			
	Sets the modulation source to external.			
Query Syntax	**SOURce[1|2]:AM:SOURce?**			
Return Parameter	INT	Internal		
	EXT	External		
Example	**SOUR1:AM:SOUR?**			
	INT			
	The modulation source is set to internal.			

SOURce[1|2]:AM:INTernal:FUNCtion

Source Specific Command

Description	Sets the shape of the modulating waveform from sine, square, triangle, upramp and dnramp. The default shape is sine.			
Note	Square and triangle waveforms have a 50% duty cycle. Upramp and dnramp have a symmetry of 100% and 0%, respectively.			
Syntax	**SOURce[1|2]:AM:INTernal:FUNCtion {SINusoid|SQUare|TRIangle|UPRamp|DNRamp}**			
Example	**SOUR1:AM:INT:FUNC SIN**			
	Sets the AM modulating wave shape to sine.			
Query Syntax	**SOURce[1|2]:AM:INTernal:FUNCtion?**			
Return Parameter	SIN	Sine	UPRAMP	Upramp
	SQU	Square	DNRAMP	Dnramp
	TRI	Triangle		
Example	**SOUR1:AM:INT:FUNC?**			
	SIN			
	The shape for the modulating waveform is Sine.			

SOURce[1|2]:AM:INTernal:FREQuency

Source Specific Command

Description	Sets the frequency of the internal modulating waveform only. The default frequency is 100Hz.	
Syntax	**SOURce[1|2]:AM:INTernal:FREQuency {<frequency>|MINimum|MAXimum}**	
Parameter	<frequency>	2 mHz~ 20 kHz
Example	**SOUR1:AM:INT:FREQ +1.0000E+02** Sets the modulating frequency to 100Hz.	
Query Syntax	**SOURce[1|2]:AM:INTernal:FREQuency? [MINimum|MAXimum]**	
Return Parameter	<NR3>	Returns the frequency in Hz.
Example	**SOUR1:AM:INT:FREQ? MIN** **+1.0000E+02** Returns the minimum frequency allowed.	

SOURce[1|2]:AM:DEPTh

Source Specific Command

Description	Sets or queries the modulation depth for internal sources only. The default is 100%.	
Note	The function generator will not output more than ±5V, regardless of the modulation depth. The modulation depth of an external source is controlled using the ±5V MOD INPUT terminal on the rear panel, and not the SOURce[1|2]:AM:DEPTh command.	
Syntax	**SOURce[1|2]:AM:DEPTh {<depth in percent>|MINimum|MAXimum}**	
Parameter	<depth in percent>	0~120%
Example	**SOUR1:AM:DEPT 50** Sets the modulation depth to 50%.	

Query Syntax	**SOURce[1|2]:AM:DEPTh? [MINimum|MAXimum]**	
Return Parameter	<NR3>	Return the modulation depth as a percentage.

Example

SOUR1:AM:DEPT?

+1.0000E+02

The modulation depth is 100%.

Frequency Modulation (FM) Commands

FM Overview

The following is an overview of the steps required to generate an FM waveform.

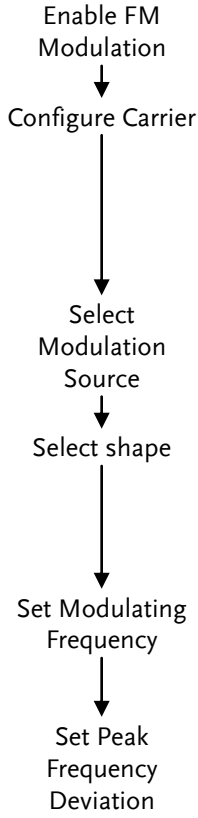

1. Turn on FM modulation using the SOURce[1|2]: FM:STAT ON command.
2. Use the APPLy command to select a carrier waveform. Alternatively, the FUNC, FREQ, AMPl, and DCOffs commands can be used to create a carrier waveform with a designated frequency, amplitude and offset.
3. Select an internal or external modulation source using the SOURce[1|2]:FM:SOUR command.
4. Use the SOURce[1|2]:FM:INT:FUNC command to select a sine, square, upramp, dnramp or triangle modulating waveshape. For internal sources only.
5. Set the modulating frequency using the SOURce[1|2]: FM:INT:FREQ command. For internal sources only.
6. Use the SOURce[1|2]:FM:DEV command to set the frequency deviation.

SOURce[1|2]:FM:STATe

Source Specific Command

Description	Sets or disables FM modulation. By default FM modulation is disabled. FM modulation must be enabled before setting other parameters.	
Note	Burst or sweep mode will be disabled if FM modulation is enabled. As only one modulation is allowed at any one time, other modulation modes will be disabled when FM modulation is enabled.	
Syntax	**SOUR[1|2]:FM:STATe {OFF|ON}**	
Example	**SOUR1:FM:STAT ON** Enables FM modulation.	
Query Syntax	**SOURce[1|2]:FM:STATe?**	
Return Parameter	0	Disabled (OFF)
	1	Enabled (ON)
Example	**SOUR1:FM:STAT?** **1** FM modulation mode is currently enabled.	

SOURce[1|2]:FM:SOURce

Source Specific Command

Description	Sets or queries the modulation source as internal or external. Internal is the default modulation source.
Note	If an external modulation source is selected, modulation depth is limited to ± 5V from the MOD INPUT terminal on the rear panel. For example, if modulation depth is set to 100%, then the maximum amplitude is +5V, and the minimum amplitude is -5V.
Syntax	**SOURce[1|2]:FM:SOURce {INTernal|EXTernal}**

Example	**SOUR1:FM:SOUR EXT** Sets the modulation source to external.			
Query Syntax	**SOURce[1|2]:FM:SOURce?**			
Return Parameter	INT	Internal		
	EXT	External		
Example	**SOUR1:FM:SOUR?** **INT** The modulation source is set to internal.			

SOURce[1|2]:FM:INTernal:FUNCtion

Source Specific Command

Description	Sets the shape of the modulating waveform from sine, square, triangle, upramp and dnramp. The default shape is sine.			
Note	Square and triangle waveforms have a 50% duty cycle. Upramp and dnramp have a symmetry of 100% and 0%, respectively.			
Syntax	**SOURce[1|2]:FM:INTernal:FUNCtion {SINusoid|SQUare|TRIangle|UPRamp|DNRamp}**			
Example	**SOUR1:FM:INT:FUNC SIN** Sets the FM modulating wave shape to sine.			
Query Syntax	**SOURce[1|2]:FM:INTernal:FUNCtion?**			
Return Parameter	SIN	Sine	UPRAMP	Upramp
	SQU	Square	DNRAMP	Dnramp
	TRI	Triangle		
Example	**SOUR1:FM:INT:FUNC?** **SIN** The shape for the modulating waveform is Sine.			

SOURce[1|2]:FM:INTernal:FREQuency

Source Specific Command

Description	Sets the frequency of the internal modulating waveform only. The default frequency is 10Hz.	
Syntax	**SOURce[1|2]:FM:INTernal:FREQuency {<frequency>|MINimum|MAXimum}**	
Parameter	<frequency>	2 mHz~ 20 kHz
Example	**SOUR1:FM:INT:FREQ 100** Sets the modulating frequency to 100Hz.	
Query Syntax	**SOURce[1|2]:FM:INTernal:FREQuency? [MINimum|MAXimum]**	
Return Parameter	<NR3>	Returns the frequency in Hz.
Example	**SOUR1:FM:INT:FREQ? MAX** **+2.0000E+04** Returns the maximum frequency allowed.	

SOURce[1|2]:FM:DEViation

Source Specific Command

Description	Sets or queries the peak frequency deviation of the modulating waveform from the carrier waveform. The default peak deviation is 100Hz. The frequency deviation of external sources is controlled using the ±5V MOD INPUT terminal on the rear panel. A positive signal (>0~+5V) will increase the deviation (up to the set frequency deviation), whilst a negative voltage will reduce the deviation.
Note	The relationship of peak deviation to modulating frequency and carrier frequency is shown below. Peak deviation = modulating frequency – carrier frequency. The carrier frequency must be greater than or

	equal to the peak deviation frequency. The sum of the deviation and carrier frequency must not exceed the maximum frequency for a specific carrier shape. If an out of range deviation is set for any of the above conditions, the deviation will be automatically adjusted to the maximum value allowed and an "out of range" error will be generated. For square wave carrier waveforms, the deviation may cause the duty cycle frequency boundary to be exceeded. In these conditions the duty cycle will be adjusted to the maximum allowed and a "settings conflict" error will be generated.	
Syntax	**SOURce[1|2]:FM:DEViation {<peak deviation in Hz>|MINimum|MAXimum}**	
Parameter	<peak deviation in Hz>	DC~25MHz DC~15MHz(square) DC~1MHz (Ramp)
Example	**SOUR1:FM:DEV MAX** Sets the frequency deviation to the maximum value allowed.	
Query Syntax	**SOURce[1|2]:FM:DEViation? [MINimum|MAXimum]**	
Return Parameter	<NR3>	Returns the frequency deviation in Hz.
Example	**SOURce[1|2]:FM:DEViation? MAX** **+1.0000E+01** Returns the maximum frequency deviation allowed.	

Frequency-Shift Keying (FSK) Commands

FSK Overview

The following is an overview of the steps required to generate an FSK modulated waveform.

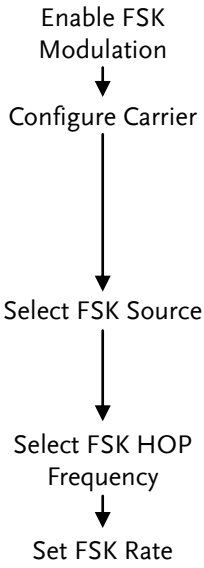

1. Turn on FSK modulation using the SOURce[1|2]: FSK:STAT ON command.
2. Use the APPLy command to select a carrier waveform. Alternatively, the FUNC, FREQ, AMPl, and DCOffs commands can be used to create a carrier waveform with a designated frequency, amplitude and offset.
3. Select an internal or external modulation source using the SOURce[1|2]:FSK:SOUR command.
4. Set the hop frequency using the SOURce[1|2]:FSK:FREQ command.
5. Use the SOURce[1|2]: FSK:INT:RATE command to set the FSK rate. The FSK rate can only be set for internal sources.

SOURce[1|2]:FSKey:STATe

Source Specific Command

Description	Turns FSK Modulation on or off. By default FSK modulation is off.
Note	Burst or sweep mode will be disabled if FSK modulation is enabled. As only one modulation is allowed at any one time, other modulation modes will be disabled when FSK modulation is enabled.
Syntax	**SOURce[1|2]:FSKey:STATe {OFF|ON}**
Example	**SOUR1:FSK:STAT ON**

	Enables FSK modulation	
Query Syntax	**SOURce[1|2]:FSKey:STATe?**	
Return Parameter	0	Disabled (OFF)
	1	Enabled (ON)
Example	**SOUR1:FSK:STAT?**	
	1	
	FSK modulation is currently enabled.	

SOURce[1|2]:FSKey:SOURce

Source Specific Command

Description	Sets or queries the FSK source as internal or external. Internal is the default source.	
Note	If an external FSK source is selected, FSK rate is controlled by the Trigger INPUT terminal on the rear panel.	
Syntax	**SOURce[1|2]:FSKey:SOURce {INTernal|EXTernal}**	
Example	**SOUR1:FSK:SOUR EXT**	
	Sets the FSK source to external.	
Query Syntax	**SOURce[1|2]:FSKey:SOURce?**	
Return Parameter	INT	Internal
	EXT	External
Example	**SOUR1:FSK:SOUR?**	
	INT	
	The FSK source is set to internal.	

SOURce[1|2]:FSKey:FREQuency

Source Specific Command

Description	Sets the FSK hop frequency. The default hop frequency is set to 100Hz.
Note	For FSK, the modulating waveform is a square wave with a duty cycle of 50%.

Syntax	**SOURce[1|2]:FSKey:FREQuency {<frequency>|MINimum|MAXimum}**	
Parameter	<frequency>	1 μHz~25MHz(sine) 1 μHz~15MHz(Square、Pulse) 1 μHz~1MHz(Ramp)
Example	**SOUR1:FSK:FREQ +1.0000E+02** Sets the FSK hop frequency to to 100Hz.	
Query Syntax	**SOURce[1|2]:FSKey:FREQuency? [MINimum|MAXimum]**	
Return Parameter	<NR3>	Returns the frequency in Hz.
Example	**SOUR1:FSK:FREQ? MAX** **+2.5000E+06** Returns the maximum hop frequency allowed.	

SOURce[1|2]:FSKey:INTernal:RATE

Source Specific Command

Description	Sets or queries the FSK rate for internal sources only.	
Note	External sources will ignore this command.	
Syntax	**SOURce[1|2]:FSKey:INTernal:RATE {<rate in Hz>|MINimum|MAXimum}**	
Parameter	<rate in Hz>	2 mHz~100 kHz
Example	**SOUR1:FSK:INT:RATE MAX** Sets the rate to the maximum (100kHz).	
Query Syntax	**SOURce[1|2]:FSKey:INTernal:RATE? [MINimum|MAXimum]**	
Return Parameter	<NR3>	Returns the FSK rate in Hz.

Example **SOUR1:FSK:INT:RATE? MAX**

+1.0000E+05

Returns the maximum FSK rate allowed.

Phase Modulation (PM)Commands

PM Overview

The following is an overview of the steps required to generate a PM modulated waveform.

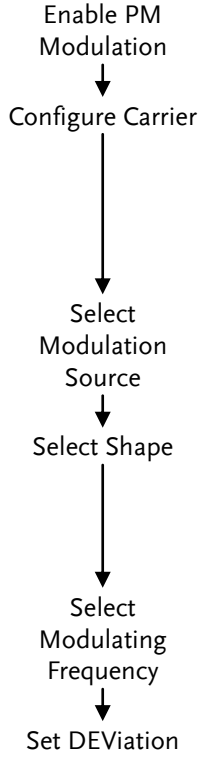

1. Turn on PM modulation using the SOURce[1|2]: PM:STATe ON command.
2. Use the APPLy command to select a carrier waveform. Alternatively, the FUNC, FREQ, AMPl, and DCOffs commands can be used to create a carrier waveform with a designated frequency, amplitude and offset.
3. Select an internal or external modulation source using the SOURce[1|2]:PM:SOUR command.
4. Use the SOURce[1|2]: PM:INT:FUNC command to select a sine, square, upramp, dnramp or triangle modulating waveshape. For internal sources only.
5. Set the modulating frequency using the SOURce[1|2]:PM:INT:FREQ command. For internal sources only.
6. Use the SOURce[1|2]:PM:DEV command to set the phase DEViation.

SOURce[1|2]:PM:STATe

Source Specific Command

Description	Turns PM Modulation on or off. By default PM modulation is off.	
Note	Burst or sweep mode will be disabled if PM modulation is enabled. As only one modulation is allowed at any one time, other modulation modes will be disabled when PM modulation is enabled.	
Syntax	**SOURce[1|2]:PM:STATe {OFF|ON}**	
Example	**SOUR1:PM:STAT ON** Enables PM modulation	
Query Syntax	**SOURce[1|2]:PM:STATe?**	
Return Parameter	0	Disabled (OFF)
	1	Enabled (ON)
Example	**SOUR1:PM:STAT?** **1** PM modulation is currently enabled.	

SOURce[1|2]:PM:SOURce

Source Specific Command

Description	Sets or queries the PM source as internal or external. Internal is the default source.	
Note	If an external PM source is selected, the phase modulation is controlled by the MOD INPUT terminal on the rear panel.	
Syntax	**SOURce[1|2]:PM:SOURce {INTernal|EXTernal}**	
Example	**SOUR1:PM:SOUR EXT** Sets the PM source to external.	
Query Syntax	**SOURce[1|2]:PM:SOURce?**	
Return Parameter	INT	Internal
	EXT	External

Example	**SOUR1:PM:SOUR?** **INT** The PM source is set to internal.

SOURce[1|2]:PM:INTernal:FUNction

Source Specific Command

Description	Sets the shape of the modulating waveform from sine, square, triangle, upramp and dnramp. The default shape is sine.
Note	Square and triangle waveforms have a 50% duty cycle. Upramp and dnramp have a symmetry to 100% and 0%, respectively. .
Syntax	**SOURce[1|2]:PM:INTernal:FUNction {SINusoid|SQUare|TRIangle|UPRamp|DNRamp}**
Example	**SOUR1:PM:INT:FUN SIN** Sets the PM modulating wave shape to sine. .
Query Syntax	**SOURce[1|2]:PM:INTernal:FUNction?**

Return Parameter				
	SIN	Sine	UPRAMP	Upramp
	SQU	Square	DNRAMP	Dnramp
	TRI	Triangle		

Example	**SOUR1:PM:INT:FUNC?** **SIN** The shape for the modulating waveform is Sine.

SOURce[1|2]:PM:INTernal:FREQuency

Source Specific Command

Description	Sets the modulating waveform frequency for internal sources. The default frequency is set to 100Hz.
Syntax	**SOURce[1|2]:PM:INTernal:FREQuency {<frequency>|MINimum|MAXimum}**

Parameter		
	<frequency>	2 mHz~ 20 kHz

Example	SOUR1:PM:INT:FREQ MAX Sets the frequency to the maximum value.	
Query Syntax	SOURce[1|2]:PM:INTernal:FREQuency?	
Return Parameter	<NR3>	Returns the frequency in Hz.
Example	SOUR1:PM:INT:FREQ? MAX +2.0000E+04 Returns the modulating frequency. (20kHz)	

SOURce[1|2]:PM:DEViation

Source Specific Command

Description	Sets or queries the phase deviation of the modulating waveform from the carrier waveform. The default phase deviation is 180°.	
Note	For external sources, the phase deviation is controlled by the ±5V MOD Input terminal on the rear panel. If the phase deviation is set to 180 degrees, then +5V represents a deviation of 180 degrees. A lower input voltage will decrease the set phase deviation.	
Syntax	SOURce[1|2]:PM:DEViation {< phase>|minimum |maximum}	
Parameter	<percent>	0°~360°
Example	SOUR1:PM:DEViation +3.0000E+01 Sets the deviation to 30°.	
Query Syntax	SOURce[1|2]:PM:DEViation?	
Return Parameter	<NR3>	Returns the deviation .
Example	SOUR1:PM:DEViation? +3.0000E+01 The current deviation is 30°.	

SUM Modulation (SUM) Commands

SUM Overview

The following is an overview of the steps required to generate a SUM modulated waveform.

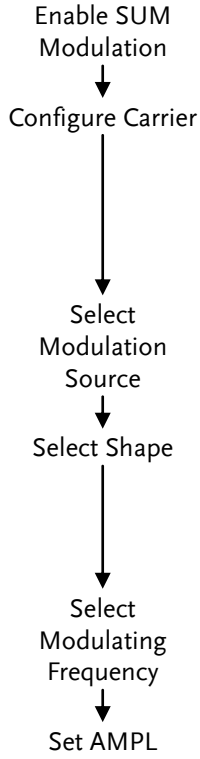

1. Turn on SUM modulation using the SOURce[1|2]: SUM:STATe ON command.
2. Use the APPLy command to select a carrier waveform. Alternatively, the FUNC, FREQ, AMPl, and DCOffs commands can be used to create a carrier waveform with a designated frequency, amplitude and offset.
3. Select an internal or external modulation source using the SOURce[1|2]:SUM:SOUR command.
4. Use the SOURce[1|2]: SUM:INT:FUNC command to select a sine, square, upramp, dnramp or triangle modulating waveshape. For internal sources only.
5. Set the modulating frequency using the SOURce[1|2]:SUM:INT:FREQ command. For internal sources only.
6. Use the SOURce[1|2]:SUM:AMPL command to set the modulating amplitude.

SOURce[1|2]:SUM:STATe

Source Specific Command

Description	Turns SUM Modulation on or off. By default SUM modulation is off.	
Note	Burst or sweep mode will be disabled if SUM modulation is enabled. As only one modulation is allowed at any one time, other modulation modes will be disabled when SUM modulation is enabled.	
Syntax	**SOURce[1|2]:SUM:STATe {OFF|ON}**	
Example	**SOUR1:SUM:STAT ON** Enables SUM modulation	
Query Syntax	**SOURce[1|2]:SUM:STATe?**	
Return Parameter	0	Disabled (OFF)
	1	Enabled (ON)
Example	**SOUR1:SUM:STAT?** **ON** SUM modulation is currently enabled.	

SOURce[1|2]:SUM:SOURce

Source Specific Command

Description	Sets or queries the SUM source as internal or external. Internal is the default source.	
Note	If an external SUM source is selected, the amplitude is controlled by the MOD INPUT terminal on the rear panel.	
Syntax	**SOURce[1|2]:SUM:SOURce {INTernal|EXTernal}**	
Example	**SOUR1:SUM:SOUR EXT** Sets the SUM source to external.	
Query Syntax	**SOURce[1|2]:SUM:SOURce?**	
Return Parameter	INT	Internal

	EXT	External

Example **SOUR1:SUM:SOUR?**

INT

The SUM source is set to internal.

SOURce[1|2]:SUM:INTernal:FUNction

Source Specific Command

Description: Sets the shape of the modulating waveform from sine, square, triangle, upramp and dnramp. The default shape is sine.

Note: Square and triangle waveforms have a 50% duty cycle. Upramp and dnramp have a symmetry to 100% and 0%, respectively. .

Syntax: **SOURce[1|2]:SUM:INTernal:FUNction {SINusoid|SQUare|TRIangle|UPRamp|DNRamp}**

Example: **SOUR1:SUM:INT:FUN SIN**

Sets the SUM modulating wave shape to sine.

Query Syntax: **SOURce[1|2]:SUM:INTernal:FUNction?**

Return Parameter				
	SIN	Sine	UPRAMP	Upramp
	SQU	Square	DNRAMP	Dnramp
	TRI	Triangle		

Example: **SOUR1:SUM:INT:FUNC?**

SIN

The shape for the modulating waveform is Sine.

SOURce[1|2]:SUM:INTernal:FREQuency

Source Specific Command

Description: Sets the modulating waveform frequency for internal sources. The default frequency is set to 100Hz.

Syntax: **SOURce[1|2]:SUM:INTernal:FREQuency {<frequency>|MINimum|MAXimum}**

Parameter	<frequency>	2 mHz~ 20 kHz
Example	SOUR1:SUM:INT:FREQ MAX Sets the frequency to the maximum value.	
Query Syntax	SOURce[1|2]:SUM:INTernal:FREQuency?	
Return Parameter	<NR3>	Returns the frequency in Hz.
Example	SOUR1:SUM:INT:FREQ? MAX +2.0000E+04 Returns the modulating frequency (20kHz).	

SOURce[1|2]:SUM:AMPL

Source Specific Command

Description	Sets or queries the amplitude of the modulating waveform from the carrier waveform. The default phase amplitude is 50%.	
Note	If an external SUM source is selected, the amplitude of the modulated waveform is controlled using the ±5V MOD INPUT terminal on the rear panel. A positive signal (>0~+5V) will increase the AMPLitude (up to the set amplitude), whilst a negative voltage will reduce the amplitude.	
Syntax	SOURce[1|2]:SUM:AMPL{< percent>|minimum |maximum}	
Parameter	<percent>	0%~100%
Example	SOUR1:SUM:AMPLitude +3.0000E+01 Sets the amplitude to 30%.	
Query Syntax	SOURce[1|2]:SUM:AMPLitude?	
Return Parameter	<NR3>	Returns the amplitude .
Example	SOUR1:SUM:AMPLitude? +3.0000E+01 The current amplitude is 30%.	

Frequency Sweep Commands

Sweep Overview

Below shows the order in which commands must be executed to perform a sweep.

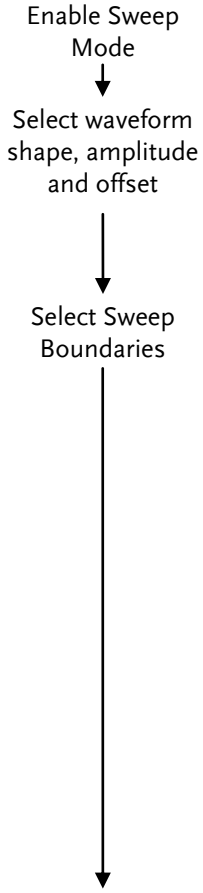

1. Turn on Sweep mode modulation using the SOURce[1|2]: SWE:STAT ON command.
2. Use the APPLy command to select the waveform shape. Alternatively, the FUNC, FREQ, AMPl, and DCOffs commands can be used to create a waveform with a designated frequency, amplitude and offset.
3. Set the frequency boundaries by setting start and stop frequencies or by setting a center frequency with a span.

   Start~Stop — Use the SOURce[1|2]:FREQ:STAR and SOURce[1|2]:FREQ:STOP to set the start and stop frequencies. To sweep up or down, set the stop frequency higher or lower than the start frequency.

   Span — Use the SOURce[1|2]:FREQ:CENT and SOURce[1|2]:FREQ:SPAN commands to set the center frequency and the frequency span. To sweep up or down, set the span as positive or negative.
4. Choose Linear or Logarithmic spacing using the SOURce[1|2]:SWE:SPAC command.

Select Sweep Time
↓
Select the sweep trigger source
↓
Select the marker frequency

5. Choose the sweep time using the SOURce[1|2]:SWE:TIME command.
6. Select an internal or external sweep trigger source using the SOURce[1|2]:SOUR command.
7. To output a marker frequency from the trigger out, use The SOURce[1|2]:MARK:FREQ command. To enable marker frequency output, use the SOURce[1|2]:MARK ON command.

The marker frequency can be set to a value within the sweep span.

SOURce[1|2]:SWEep:STATe

Source Specific Command

Description	Sets or disables Sweep mode. By default Sweep is disabled. Sweep modulation must be enabled before setting other parameters.	
Note	Any modulation modes or Burst mode will be disabled if sweep mode is enabled.	
Syntax	**SOURce[1|2]:SWEep:STATe {OFF|ON}**	
Example	**SOUR1:SWE:STAT ON** Enables sweep mode.	
Query Syntax	**SOURce[1|2]:SWEep:STATe?**	
Return Parameter	0	Disabled (OFF)
	1	Enabled (ON)
Example	**SOUR1:SWE:STAT?** **1** Sweep mode is currently enabled.	

SOURce[1|2]:FREQuency:STARt

Source Specific Command

Description	Sets the start frequency of the sweep. 100Hz is the default start frequency.	
Note	To sweep up or down, set the stop frequency higher or lower than the start frequency.	
Syntax	**SOURce[1|2]:FREQuency:STARt {<frequency>|MINimum|MAXimum}**	
Parameter	<frequency>	1μHz~ 25MHz 1μHz~ 15MHz(Square) 1μHz~ 1MHz (Ramp)
Example	**SOUR1:FREQ:STAR +2.0000E+03** Sets the start frequency to 2kHz.	
Query Syntax	**SOURce[1|2]:FREQuency:STARt? [MINimum|MAXimum]**	
Return Parameter	<NR3>	Returns the start frequency in Hz.
Example	**SOUR1:FREQ:STAR? MAX** **+8.0000E+0** Returns the maximum start frequency allowed.	

SOURce[1|2]:FREQuency:STOP

Source Specific Command

Description	Sets the stop frequency of the sweep. 1 kHz is the default start frequency.
Note	To sweep up or down, set the stop frequency higher or lower than the start frequency.
Syntax	**SOURce[1|2]:FREQuency:STOP {<frequency>|MINimum|MAXimum}**

Parameter	<frequency>	1μHz~ 25MHz 1μHz~ 15MHz(Square) 1μHz~ 1MHz (Ramp)
Example	**SOUR1:FREQ:STOP +2.0000E+03** Sets the stop frequency to 2kHz.	
Query Syntax	**SOURce[1|2]:FREQuency:STOP? [MINimum|MAXimum]**	
Return Parameter	<NR3>	Returns the stop frequency in Hz.
Example	**SOUR1:FREQ:STOP? MAX** **+8.0000E+00** Returns the maximum stop frequency allowed.	

SOURce[1|2]:FREQuency:CENTer

Source Specific Command

Description	Sets and queries the center frequency of the sweep. 550 Hz is the default center frequency.	
Note	The maximum center frequency depends on the sweep span and maximum frequency: max center freq = max freq – span/2	
Syntax	**SOURce[1|2]:FREQuency:CENTer {<frequency>|MINimum|MAXimum}**	
Parameter	<frequency>	450Hz~ 25MHz 450Hz~ 15MHz(Square) 450Hz~ 1MHz (Ramp)
Example	**SOUR1:FREQ:CENT +2.0000E+03** Sets the center frequency to 2kHz.	
Query Syntax	**SOURce[1|2]:FREQuency:CENTer? [MINimum|MAXimum]**	
Return Parameter	<NR3>	Returns the stop frequency in Hz.

Example	**SOUR1:FREQ:CENT? MAX** **+8.0000E+00** Returns the maximum center frequency allowed, depending on the span.

SOURce[1|2]:FREQuency:SPAN

Source Specific Command

Description	Sets and queries the frequency span of the sweep. 900 Hz is the default frequency span. The span frequency is equal to the stop-start frequencies.	
Note	To sweep up or down, set the span as positive or negative. The maximum span frequency has a relationship to the center frequency and maximum frequency: max freq span= 2(max freq – center freq)	
Syntax	**SOURce[1|2]:FREQuency:SPAN {<frequency>|MINimum|MAXimum}**	
Parameter	<frequency>	+/-1μHz~+/- 25MHz +/-1μHz~+/-15MHz(Squa) +/-1μHz~ +/-1MHz (Ramp)
Example	**SOUR1:FREQ:SPAN +2.0000E+03** Sets the frequency span to 2kHz.	
Query Syntax	**SOURce[1|2]:FREQuency:SPAN? [MINimum| MAXimum]**	
Return Parameter	<NR3>	Returns the frequency span in Hz.
Example	**SOUR1:FREQ:SPAN?** **+2.0000E+03** Returns the frequency span for the current sweep.	

SOURce[1|2]:SWEep:SPACing

Source Specific Command

Description	Sets linear or logarithmic sweep spacing. The default spacing is linear.	
Syntax	**SOURce[1|2]:SWEep:SPACing {LINear|LOGarithmic}**	
Example	**SOUR1:SWE:SPAC LIN** Sets the spacing to linear.	
Query Syntax	**SOURce[1|2]:SWEep:SPACing?**	
Return Parameter	LIN	Linear spacing
	LOG	Logarithmic spacing
Example	**SOUR1:SWE:SPAC?** **LIN** The spacing is currently set as linear.	

SOURce[1|2]:SWEep:TIME

Source Specific Command

Description	Sets or queries the sweep time. The default sweep time is 1 second.	
Note	The function generator automatically determines the number of frequency points that are used for the sweep based on the sweep time.	
Syntax	**SOURce[1|2]:SWEep:TIME {<seconds>|MINimum|MAXimum}**	
Parameter	<seconds>	1 ms ~ 500 s
Example	**SOUR1:SWE:TIME +1.0000E+00** Sets the sweep time to 1 second.	
Query Syntax	**SOURce[1|2]:SWEep:TIME? {<seconds>|MINimum|MAXimum}**	
Return Parameter	<NR3>	Returns sweep time in seconds.

Example	**SOUR1:SWE:TIME?** **+2.0000E+01** Returns the sweep time (20 seconds).

SOURce[1|2]:SWEep:SOURce

Source Specific Command

Description	Sets or queries the trigger source as immediate (internal), external or manual. Immediate (internal) is the default trigger source. IMMediate will constantly output a swept waveform. EXTernal will output a swept waveform after each external trigger pulse. Manual will ouput a swept waveform after the trigger softkey is pressed.	
Note	If the APPLy command was used to create the waveform shape, the source is automatically set to IMMediate. The *OPC/*OPC? command/query can be used to signal the end of the sweep.	
Syntax	**SOURce[1|2]: SWEep:SOURce {IMMediate|EXTernal|MANual}**	
Example	**SOUR1: SWE:SOUR EXT** Sets the sweep source to external.	
Query Syntax	**SOURce[1|2]: SWEep:SOURce?**	
Return Parameter	IMM	Immediate
	EXT	External
	MANual	Manual
Example	**SOUR1:SWE:SOUR?** **IMM** The sweep source is set to immediate.	

SOURce[1|2]:MARKer:FREQuency

Source Specific Command

Description	Sets or queries the marker frequency. The default marker frequency is 550 Hz. The marker frequency is used to output a trigger out signal from the trigger terminal on the rear panel.	
Note	The marker frequency must be between the start and stop frequencies. If the marker frequency is set to a value that is out of the range, the marker frequency will be set to the center frequency and a "settings conflict" error will be generated.	
Syntax	**SOURce[1|2]:MARKer:FREQuency {<frequency>|MINimum|MAXimum}**	
Parameter	<frequency>	1μHz ~ 25 MHz 1 μHz ~ 1 MHz (Ramp)
Example	**SOUR1:MARK:FREQ +1.0000E+03** Sets the marker frequency to 1 kHz.	
Query Syntax	**SOURce[1|2]:MARKer:FREQuency? [MINimum|MAXimum]**	
Return Parameter	<NR3>	Returns the marker frequency in Hz.
Example	**SOUR1:MARK:FREQ? MAX** **+1.0000E+03** Returns the marker frequency (1 kHz).	

SOURce[1|2]:MARKer

Source Specific Command

Description	Turns the marker frequency on or off. The default is off.	
Note	MARKer ON	The SYNC signal goes logically high/low at the start of each sweep and goes low/high at the marker frequency.

	MARKer OFF The SYNC signal turn off	
Syntax	**SOURce[1|2]:MARKer {OFF|ON}**	
Example	**SOUR1:MARK ON**	
	Enables the marker frequency.	
Query Syntax	**SOURce[1|2]:MARKer?**	
Return Parameter	0	Disabled
	1	Enabled
Example	**SOUR1:MARK?**	
	1	
	The marker frequency is enabled.	

Burst Mode Commands

Burst Mode Overview

Burst mode can be configured to use an internal trigger (N Cycle mode) or an external trigger (Gate mode) using the Trigger INPUT terminal on the rear panel. Using N Cycle mode, each time the function generator receives a trigger, the function generator will output a specified number of waveform cycles (burst). After the burst, the function generator will wait for the next trigger before outputting another burst. N Cycle is the default Burst mode.

The alternative to using a specified number of cycles, Gate mode uses the external trigger to turn on or off the output. When the Trigger INPUT signal is high*, waveforms are continuously output (creating a burst). When the Trigger INPUT signal goes low*, the waveforms will stop being output after the last waveform completes its period. The voltage level of the output will remain equal to the starting phase of the burst waveforms, ready for the signal to go high* again.

*assuming the Trigger polarity is not inverted.

Only one burst mode can be used at any one time. The burst mode depends on the source of the trigger (internal, external, manual) and the source of the burst.

	Function		
Burst Mode & Source	N Cycle*	Cycle	Phase
Triggered – IMMediate, BUS	Available	Available	Available
Triggered - EXTernal, MANual	Available	Unused	Available
Gated pulse - IMMediate	Unused	Unused	Available

*burst count

The following is an overview of the steps required to generate a burst waveform.

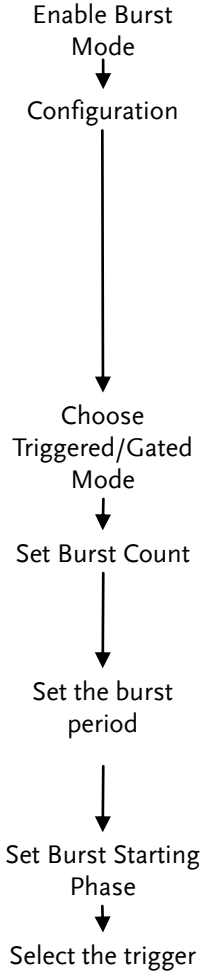

1. Turn on Burst mode using the SOURce[1|2]:BURS:STAT ON command.
2. Use the APPLy command to select a sine, square, ramp, pulse burst waveform*. Alternatively, the FUNC, FREQ, AMPl, and DCOffs commands can be used to create the burst waveform* with a designated frequency, amplitude and offset.

   *2 mHz minimum for internally triggered bursts.
3. Use the SOURce[1|2]: BURS:MODE command to select from triggered or gated burst modes.
4. Use the SOURce[1|2]:BURS:NCYC command to set the burst count. This command is only for triggered burst mode only.
5. Use the SOURce[1|2]:BURS:INT:PER command to set the burst period/cycle. This command is only applicable for triggered burst mode (internal trigger).
6. Use the SOURce[1|2]:BURS:PHAS command to set the burst starting phase.
7. Use the SOURce[1|2]:BURS:TRIG:SOUR command to select the trigger source for triggered burst mode only.

SOURce[1|2]:BURSt:STATe

Source Specific Command

Description	Turns burst mode on or off. By default burst mode is turned off.	
Note	When burst mode is turned on, sweep and any modulation modes are disabled.	
Syntax	**SOURce[1|2]:BURSt:STATe {OFF|ON}**	
Example	**SOUR1:BURS:STAT ON** Turns burst mode on.	
Query Syntax	**SOURce[1|2]:BURSt:STATe?**	
Return Parameter	0	Disabled
	1	Enabled
Example	**SOUR1:BURS:STAT?** **0** Burst mode is off.	

SOURce[1|2]:BURSt:MODE

Source Specific Command

Description	Sets or queries the burst mode as gated or triggered. The default burst mode is triggered.	
Note	The burst count, period, trigger source and any manual trigger commands are ignored in gated burst mode.	
Syntax	**SOURce[1|2]:BURSt:MODE {TRIGgered|GATed}**	
Example	**SOUR1:BURS:MODE TRIG** Sets the burst mode to triggered.	
Query Syntax	**SOURce[1|2]:BURSt:MODE?**	
Return Parameter	TRIG	Triggered mode
	GAT	Gated mode

Example	SOUR1:BURS:MODE? TRIG The current burst mode is triggered.

SOURce[1|2]:BURSt:NCYCles

Source Specific Command

Description	Sets or queries the number of cycles (burst count) in triggered burst mode. The default number of cycles is 1. The burst count is ignored in gated mode.	
Note	If the trigger source is set to immediate, the product of the burst period and waveform frequency must be greater than the burst count: Burst Period X Waveform frequency > burst count If the burst count is too large, the burst period will automatically be increased and a "Settings conflict" error will be generated. Only sine and square waves are allowed infinite burst above 15 MHz.	
Syntax	**SOURce[1|2]:BURSt:NCYCles{< # cycles> |INFinity|MINimum |MAXimum}**	
Parameter	<# cycles>	1~65535 cycles.
	INFinity	Sets the number to continuous.
	MINimum	Sets the number to minimum allowed.
	MAXimum	Sets the number to maximum allowed.
Example	**SOUR1:BURS:NCYCl INF** Sets the number of burst cycles to continuous (infinite).	
Query Syntax	**SOURce[1|2]:BURSt:NCYCles? [MINimum|MAXimum]**	
Return Parameter	<NR3>	Returns the number of cycles.
	INF	INF is returned if the number of cycles is continuous.

Example	SOUR1:BURS:NCYC? +1.0000E+02 The burst cycles are set to 100.

SOURce[1|2]:BURSt:INTernal:PERiod

Source Specific Command

Description	Sets or queries the burst period. Burst period settings are only applicable when the trigger is set to immediate. The default burst period is 10 ms. During manual triggering, external triggering or Gate burst mode, the burst period settings are ignored.
Note	The burst period must be long enough to output the designated number of cycles for a selected frequency. Burst period > burst count/(waveform frequency + 200 ns) If the period is too short, it is automatically increased so that a burst can be continuously output. A "data out of range" error will also be generated.
Syntax	SOURce[1|2]:BURSt:INTernal:PERiod {<seconds>|MINimum|MAXimum}
Parameter	<seconds > 1 ms ~ 500 seconds
Example	SOUR1:BURS:INT:PER +1.0000E+01 Sets the period to 10 seconds.
Query Syntax	SOURce[1|2]:BURSt:INTernal:PERiod? [MINimum|MAXimum]
Return Parameter	<NR3> Returns the burst period in seconds.
Example	SOUR1:BURS:INT:PER? +1.0000E+01 The burst period is 10 seconds.

SOURce[1|2]:BURSt:PHASe

Source Specific Command

Description	Sets or queries the starting phase for the burst. The default phase is 0 degrees. At 0 degrees, sine square and ramp waveforms are at 0 volts. In gated burst mode, waveforms are continuously output (burst) when the Trig signal is true. The voltage level at the starting phase is used to determine the voltage level of the signal in-between bursts.
Note	The phase command is not used with pulse waveforms.
Syntax	**SOURce[1|2]:BURSt:PHASe {<angle>|MINimum|MAXimum}**
Parameter	<angle> -360 ~ 360 degrees
Example	**SOUR1:BURS:PHAS MAX** Sets the phase to 360 degrees.
Query Syntax	**SOURce[1|2]:BURSt:PHASe? [MINimum|MAXimum]**
Return Parameter	<NR3> Returns the phase angle in degrees.
Example	**SOUR1:BURS:PHAS?** **+1.2000E+02** The burst phase is 120 degrees.

SOURce[1|2]:BURSt:TRIGger:SOURce

Source Specific Command

Description	Sets or queries the trigger source for triggered burst mode. In trigged burst mode, a waveform burst is output each time a trigger signal is received and the number of cycles is determined by the burst count. There are three trigger sources for triggered burst mode:

	Immediate	A burst is output at a set frequency determined by the burst period.
	External	EXTernal will output a burst waveform after each external trigger pulse. Any additional trigger pulse signals before the end of the burst are ignored.
	Manual	Manual triggering will output a burst waveform after the trigger softkey is pressed.
Note	If the APPLy command was used, the source is automatically set to IMMediate. The *OPC/*OPC? command/query can be used to signal the end of the burst.	
Syntax	**SOURce[1|2]:BURSt:TRIGger:SOURce {IMMediate|EXTernal|MANual}**	
Example	**SOUR1:BURS:TRIG:SOUR EXT** Sets the burst trigger source to external.	
Query Syntax	**SOURce[1|2]:BURSt:TRIGger:SOURce?**	
Return Parameter	IMM	Immediate
	EXT	External
	MANual	Manual
Example	**SOUR1:BURS:TRIG:SOUR?** **IMM** The burst trigger source is set to immediate.	

SOURce[1|2]:BURSt:TRIGger:DELay

Source Specific Command

Description	The DELay command is used to insert a delay (in seconds) before a burst is output. The delay starts after a trigger is received. The default delay is 0 seconds.

Syntax	**SOURce[1|2]: BURSt:TRIGger:DELay {<seconds>|MINimum|MAXimum}**	
Parameter	<seconds>	0~655350 nS
Example	**SOUR1:BURS:TRIG:DEL +1.0000E+01** Sets the trigger delay to 10 seconds.	
Query Syntax	**SOURce[1|2]:BURSt:TRIGger:DELay? [MINimum|MAXimum]**	
Return Parameter	<NRf>	Delay in seconds
Example	**SOUR1:BURS:TRIG:DEL ?** **+1.0000E+01** The trigger delay is 10 seconds.	

SOURce[1|2]:BURSt:TRIGger:SLOPe

Source Specific Command

Description	Sets or queries the trigger edge for externally triggered bursts from the Trigger INPUT terminal on the rear panel. By default the trigger is rising edge (Positive).	
Syntax	**SOURce[1|2]:BURSt:TRIGger:SLOPe {POSitive|NEGative}**	
Parameter	POSitive	rising edge
	NEGative	falling edge
Example	**SOUR1:BURS:TRIG:SLOP NEG** Sets the trigger slope to negative.	
Query Syntax	**SOURce[1|2]:BURSt:TRIGger:SLOPe?**	
Return Parameter	POS	rising edge
	NEG	falling edge
Example	**SOUR1:BURS:TRIG:SLOP ?** **NEG** The trigger slope is negative.	

SOURce[1|2]:BURSt:TRIGger:MANual

Source Specific Command

Description	This command is used to manually trigger a burst waveform when the source trigger is set to manual for the selected channel. This command is the equivalent of pressing the trigger soft-key on the front panel for manual triggering.
Syntax	**SOURce[1|2]:BURSt:TRIGger:MANual**
Example	**SOUR1:BURS:TRIG:MAN** Manually triggers the burst waveform.

SOURce[1|2]:BURSt:GATE:POLarity

Source Specific Command

Description	In gated mode, the function generator will output a waveform continuously while the external trigger receives logically true signal from the Trigger INPUT terminal. Normally a signal is logically true when it is high. The logical level can be inverted so that a low signal is considered true.	
Syntax	**SOURce[1|2]:BURSt:GATE:POLarity {NORMal|INVertes}**	
Parameter	NORMal	Logically high
	INVertes	Logically low
Example	**SOUR1:BURS:GATE:POL INV** Sets the state to logically low (inverted).	
Query Syntax	**SOURce[1|2]:BURSt:GATE:POLarity?**	
Return Parameter	NORM	Normal(High) logical level
	INV	Inverted (low) logical level
Example	**SOUR1:BURS:GATE:POL?** **INV** The true state is inverted(logically low).	

SOURce[1|2]:BURSt:OUTPut:TRIGger:SLOPe

Source Specific Command

Description	Sets or queries the trigger edge of the trigger output signal. The signal is output from the trigger out terminal on the rear panel. The default trigger output slope is positive.	
	Immediate	50% duty cycle square wave is output at the start of each burst.
	External	Trigger output disabled.
	Gated mode	Trigger output disabled.
	Manual	A >1 ms pulse is output at the start of each burst.
Syntax	**SOURce[1|2]:BURSt:OUTPut:TRIGger:SLOPe {POSitive|NEGative}**	
Parameter	POSitive	Rising edge.
	NEGative	Falling edge.
Example	**SOUR1:BURS:OUTP:TRIG:SLOP POS**	
	Sets the trigger output signal slope to positive (rising edge).	
Query Syntax	**SOURce[1|2]:BURSt:OUTPut:TRIGger:SLOPe?**	
Return Parameter	POS	Rising edge.
	NEG	Falling edge.
Example	**SOUR1:BURS:OUTP:TRIG:SLOP?**	
	POS	
	The trigger output signal slope to positive.	

OUTPut[1|2]:TRIGger

Source Specific Command

Description	Sets or queries the trigger output signal on or off. By default the signal is disabled. When enabled, a TTL compatible square wave is output.	
Syntax	**OUTPut[1|2]:TRIGger {OFF|ON}**	
Parameter	OFF	Turns the output off.
	ON	Turns the output on.
Example	**OUTP1:TRIG ON** Turns the output on.	
Query Syntax	**OUTPut[1|2]:TRIGger?**	
Return Parameter	0	Disabled
	1	Enabled
Query Example	**OUTP1:TRIG?** **1** The trigger output is enabled.	

Arbitrary Waveform Commands

Arbitrary Waveform Overview

Use the steps below to output an arbitrary waveform over the remote interface.

Output Arbitrary Waveform
↓
Select Waveform Frequency, amplitude and offset
↓
Load Waveform Data
↓
Set Waveform Rate

1. Use the SOURce[1|2]:FUNCtion USER command to output the arbitrary waveform currently selected in memory.
2. Use the APPLy command to select frequency, amplitude and DC offset. Alternatively, the FUNC, FREQ, AMPl, and DCOffs commands can be used.
3. Waveform data (1 to 4096 points per waveform) can be downloaded into volatile memory using the SOURce[1|2]:DATA:DAC command. Binary integer or decimal integer values in the range of ± 511 can be used.
4. The waveform rate is the product of the number of points in the waveform and the waveform frequency.

Rate = Hz × # points

Range:	Rate:	120MHz
	Frequency:	60MHz
	# points:	1~4096

SOURce[1|2]:FUNCtion USER

Source Specific Command

Description	Use the SOURce[1|2]:FUNCtion USER command to output the arbitrary waveform currently selected in memory. The waveform is output with the current frequency, amplitude and offset settings.
Syntax	**SOURce[1|2]:FUNCtion USER**
Example	**SOUR1:FUNC USER** Selects and outputs the current waveform in memory.

SOURce[1|2]:DATA:DAC

Source Specific Command

Description	The SOURce[1|2]:DATA:DAC command is used to download binary or decimal integer values into memory using the IEEE-488.2 binary block format or as an ordered list of values.
Note	The integer values (±511) correspond to the maximum and minimum peak amplitudes of the waveform. For instance, for a waveform with an amplitude of 5Vpp (0 offset), the value 511is the equivalent of 2.5 Volts. If the integer values do not span the full output range, the peak amplitude will be limited. The IEEE-488.2 binary block format is comprised of three parts:  1. Initialization character (#) 2. Digit length (in ASCII) of the number of bytes 3. Number of bytes IEEE 488.2 uses two bytes to represent waveform

	data (16 bit integer). Therefore the number of bytes is always twice the number of data points.	
Syntax	**SOURce[1|2]:DATA:DAC VOLATILE, <start>, {<binary block>|<value>, <value>, . . . }**	
Parameter	<start>	Start address of the arbitrary waveform
	<binary block>	
	<value>	Decimal or integer values ±511
Example	**SOURce[1|2]:DATA:DAC VOLATILE, #210 Binary Data** The command above downloads 5 data values (stored in 16 bytes) using the binary block format. **SOURce[1|2]:DATA:DAC VOLATILE, 1000, 511, 200, 0, -200, -511** Downloads the data values (511, 200, 0, -200, -511) to address 1000.	

SOURce[1|2]:ARB:EDIT:COPY

Source Specific Command

Description	Copies a segment of a waveform to a specific starting address.	
Syntax	**SOURce[1|2]:ARB:EDIT:COPY [<start>[,<length>[,<paste>]]]**	
Parameter	<start>	Start address: 0~4095
	<length>	1 ~ 4096
	<paste>	Paste address: 0~4095
Example	**SOUR1:ARB:EDIT:COPY 1000, 256, 1257** Copies 256 data values starting at address 1000 and copies them to address 1257.	

SOURce[1|2]:ARB:EDIT:DELete

Source Specific Command

Description	Deletes a segment of a waveform from memory. The segment is defined by a starting address and length.	
Note	A waveform/waveform segment cannot be deleted when output.	
Syntax	**SOURce[1|2]:ARB:EDIT:DELete [<STARt>[,<LENGth>]]**	
Parameter	<STARt>	Start address: 0~4095
	<LENGth>	1 ~ 4096
Example	**SOURce1:ARB:EDIT:DEL 1000, 256**	
	Deletes a section of 256 data points from the waveform starting at address 1000.	

SOURce[1|2]:ARB:EDIT:DELete:ALL

Source Specific Command

Description	Deletes all user-defined waveforms from non-volatile memory and the current waveform in volatile memory.
Note	A waveform cannot be deleted when output.
Syntax	**SOURce[1|2]:ARB:EDIT:DELete:ALL**
Example	**SOUR1:ARB:EDIT:DEL:ALL**
	Deletes all user waveforms from memory.

SOURce[1|2]:ARB:EDIT:POINt

Source Specific Command

Description	Edit a point on the arbitrary waveform.	
Note	A waveform/waveform segment cannot be deleted when output.	
Syntax	**SOURce[1|2]:ARB:EDIT:POINt [<address> [, <data>]]**	
Parameter	<address>	Address of data point: 0~4095

	<data>	Value data: ± 511
Example	**SOUR1:ARB:EDIT:POIN 1000, 511** Creates a point on the arbitrary waveform at address 1000 with the highest amplitude.	

SOURce[1|2]:ARB:EDIT:LINE

Source Specific Command

Description	Edit a line on the arbitrary waveform. The line is created with a starting address and data point and a finishing address and data point.	
Note	A waveform/waveform segment cannot be deleted when output.	
Syntax	**SOURce[1|2]:ARB:EDIT:LINE [<address1>[,<data>[,<address2>[,<data2>]]]]**	
Parameter	<addrress1>	Address of data point1: 0~4095
	<data1>	Value data2: ± 511
	<address2>	Address of data point2: 0~4095
	<data2>	Value data2: ± 511
Example	**SOUR1:ARB:EDIT:LINE 40, 50, 100, 50** Creates a line on the arbitrary waveform at 40,50 to 100,50.	

SOURce[1|2]:ARB:EDIT:PROTect

Source Specific Command

Description	Protects a segment of the arbitrary waveform from deletion or editing.	
Syntax	**SOURce[1|2]:ARB:EDIT:PROTect [<STARt>[,<LENGth>]**	
Parameter	<STARt>	Start address: 0~4095
	<LENGth>	1 ~ 4096
Example	**SOUR1:ARB:EDIT:PROT 40, 50**	

Protects a segment of the waveform from address 40 for 50 data points.

SOURce[1|2]:ARB:EDIT:PROTect:ALL

Source Specific Command

Description	Protects the arbitrary waveform currently in non-volatile memory/ currently being output.
Syntax	**SOURce[1|2]:ARB:EDIT:PROTect:ALL**
Example	**SOUR1:ARB:EDIT:PROT:ALL**

SOURce[1|2]:ARB:EDIT:UNProtect

Source Specific Command

Description	Uprotects the arbitrary waveform currently in non-volatile memory/currently being output.
Syntax	**SOURce[1|2]:ARB:EDIT:UNProtect**
Example	**SOUR1:ARB:EDIT:UNP**

SOURce[1|2]:ARB:OUTPut

Source Specific Command

Description	Output the current arbitrary waveform in volatile memory. A specified start and length can also be designated.	
Syntax	**SOURce[1|2]:ARB:OUTPut [<STARt>[,<LENGth>]]**	
Parameter	<STARt>	Start address*: 0~4096
	<LENGth>	Length*: 0 ~ 4096
	* Start + Length ≤ currently output arbitrary waveform	
Example	**SOUR1:ARB:OUTP 20,200**	
	Outputs the current arbitrary waveform in memory.	

COUNTER

The frequency counter function can be turned on remotely to control the frequency counter.

COUNTER:STATE

Instrument Command

Description	Turns the frequency counter function on or off.	
Syntax	**COUNter:STATe {ON|OFF}**	
Example	**COUNter:STATe ON**	
	Turns the frequency counter on	
Query Syntax	**COUNter:STATe?**	
Return Parameter	1	ON
	0	OFF
Example	**COUNter:STATe?**	
	1	
	Turns on the frequency counter.	

COUNter:GATe

Instrument Command

Description	Sets the gate time for the frequency counter.
Syntax	**COUNter:GATe {0.01|0.1|1|10}**
Example	**COUNter:GATe 1**
	Sets the gate time to 1S.
Syntax	**COUNter:GATe? {max|min}**
Example	**COUNter:GATe?**
	1
	Returns the gate time: 1S.

COUNter:VALue?	Instrument Command

Description	Returns the current value from the frequency counter.
Syntax	COUNter:VALue?
Example	**COUNter:VALue?** +5.00E+02 Returns the frequency as 500Hz.

PHASE

The phase command remotely controls the phase and channel synchronization.

SOURce[1|2]:PHASe	Instrument Command

Description	Sets the phase.	
Syntax	**SOURce[1|2]:PHASe {<phase>|<MIN>|<MAX>}**	
Parameter	phase	-180~180
	min	Sets the phase to the minimum value.
	max	Sets the phase to the maxium value.
Example	**SOURce1:PHASe 25** Sets the phase of channel 1 to 25°.	
Query Syntax	**SOURce[1|2]:PHASe? {MAX|MIN}**	
Return Parameter	phase	Returns the current phase.
Example	**SOURce1:PHASe?** 26 Returns the phase of channel 1 as 26°.	

SOURce[1|2]:PHASe:SYNChronize	Instrument Command

Description	Sychronizes the phase of channel 1 and channel 2. SOURce1 or SOURce2 has not effect on this command.
Syntax	SOURce[1|2]:PHASe:SYNChronize
Example	SOURce1:PHASe:SYNChronize Synchronizes the phase of channel 1 and channel 2.

COUPLE

The Couple commands can be used to remotely set the frequency coupling and amplitude coupling.

SOURce[1|2]:FREQuency:COUPle:MODE	Instrument Command

Description	Set the frequency coupling mode.	
Syntax	**SOURce[1|2]:FREQuency:COUPle:MODE {Off|Offset|Ratio}**	
Example	**SOURce1:FREQuency:COUPle:MODE Offset** Sets the frequency coupling mode to offset.	
Query Syntax	**SOURce[1|2]:FREQuency:COUPle:MODE?**	
Return Parameter	Off	Disables frequency coupling.
	Offset	Set frequency coupling to offset mode.
	Ratio	Sets frequency coupling to ratio mode.
Example	**SOURce1:FREQuency:COUPle:MODE?** Off Frequency coupling is turned off.	

SOURce[1|2]:FREQuency:COUPle:OFFSet

Instrument Command

Description	Sets the offset frequency when the frequency coupling mode is set to offset.
Syntax	**SOURce[1|2]:FREQuency:COUPle:OFFSet {frequency}**
Example	**SOURce1:FREQuency:COUPle:OFFSet 2khz** Sets the offset frequency to 2kHz (the frequency of CH2 minus CH1 is 2kHz).
Syntax	**SOURce[1|2]:FREQuency:COUPle:OFFSet?**
Example	**SOURce1:FREQuency:COUPle:OFFSet?** +2.0000E+03 The offset of channel 2 from channel 1 is 2kHz.

SOURce[1|2]:FREQuency:COUPle:RATio

Instrument Command

Description	Sets the frequency coupling ratio when frequency coupling is set to ratio mode.
Syntax	**SOURce[1|2]:FREQuency:COUPle:RATio {ratio}**
Example	**SOURce1:FREQuency:COUPle:RATio 2** Set the CH2 to CH1 frequency ratio to 2.
Query Syntax	**SOURce[1|2]:FREQuency:COUPle:RATio?**
Example	**SOURce1:FREQuency:COUPle:RATio?** +2.0000E+00 Returns the CH2 to CH1 frequency ratio as 2.

SOURce[1|2]:AMPlitude:COUPle:STATe

Instrument Command

Description	Enables or disables the amplitude coupling.
Syntax	SOURce[1|2]:AMPlitude:COUPle:STATe {ON|Off}

Example	**SOURce1:AMPlitude:COUPle:STATe on**	
Description	Turns amplitude coupling on.	
Query Syntax	**SOURce[1|2]:AMPlitude:COUPle:STATe?**	
Return Parameter	1	ON
	0	Off
Example	**SOURce1:AMPlitude:COUPle:STATe?**	
	1	
	Amplitude coupling has been enabled.	

SOURce[1|2]:TRACk

Instrument Command

Description	Turns tracking on or off.	
Syntax	**SOURce[1|2]:TRACk {ON|OFF|INVerted}**	
Example	**SOURce1:TRACk ON**	
	Turns tracking on. Channel 2 will "track" the changes of channel 1.	
Query Syntax	**SOURce[1|2]:TRACk?**	
Return Parameter	ON	ON
	OFF	OFF
	INV	INVerted
Example	**SOURce1:TRACk?**	
	ON	
	Channel tracking is turned on.	

Save and Recall Commands

Up to 10 different instrument states can be stored to non-volatile memory (memory locations 0~9).

*SAV	Instrument Command
Description	Saves the current instrument state to a specified save slot. When a state is saved, all the current instrument settings, functions and waveforms are also saved.
Note	The *SAV command doesn't save waveforms in non-volatile memory, only the instrument state. The *RST command will not delete saved instrument states from memory.
Syntax	***SAV {0|1|2|3|4|5|6|7|8|9}**
Example	***SAV 0** Save the instrument state to memory location 0.

*RCL	Instrument Command
Description	Recall previously saved instrument states from memory locations 0~9.
Syntax	***RCL {0|1|2|3|4|5|6|7|8|9}**
Example	***RCL 0** Recall instrument state from memory location 0.

MEMory:STATe:DELete	Instrument Command
Description	Delete memory from a specified memory location.
Syntax	**MEMory:STATe:DELete {0|1|2|3|4|5|6|7|8|9}**
Example	**MEM:STAT:DEL 0**

Delete instrument state （ARB+Setting） from memory location 0.

MEMory:STATe:DELete ALL	Instrument Command
Description	Delete memory from all memory locations, 0~9.
Syntax	**MEMory:STATe:DELete ALL**
Example	**MEM:STAT:DEL ALL** Deletes all the instrument states from memory locations 0~9.

Error Messages

The AFG-2225 has a number of specific error codes. Use the SYSTem:ERRor command to recall the error codes. For more information regarding the error queue.

Command Error Codes

-101 Invalid character

An invalid character was used in the command string. Example: #, $, %.

SOURce1:AM:DEPTh MIN%

-102 Syntax error

Invalid syntax was used in the command string. Example: An unexpected character may have been encountered, like an unexpected space.

SOURce1:APPL:SQUare , 1

-103 Invalid separator

An invalid separator was used in the command string. Example: a space, comma or colon was incorrectly used.

APPL:SIN 1 1000 OR SOURce1:APPL:SQUare

-108 Parameter not allowed

The command received more parameters than were expected. Example: An extra (not needed) parameter was added to a command

SOURce1:APPL? 10

-109 Missing parameter

The command received less parameters than expected. Example: A required parameter was omitted.

SOURce1:APPL:SQUare

-112 Program mnemonic too long

A command header contains more than 12 characters:

OUTP:SYNCHRONIZATION ON

-113 Undefined header

An undefined header was encountered. The header is syntactically correct. Example: the header contains a character mistake.

SOUR1:AMM:DEPT MIN

-123 Exponent too large

Numeric exponent exceeds 32,000. Example:

SOURce[1|2]:BURSt:NCYCles 1E34000

-124 Too many digits

The mantissa (excluding leading 0's) contains more than 255 digits.

-128 Numeric data not allowed

An unexpected numeric character was received in the command. Example: a numeric parameter is used instead of a character string.

SOURce1:BURSt:MODE 123

-131 Invalid suffix

An invalid suffix was used. Example: An unknown or incorrect suffix may have been used with a parameter.

SOURce1:SWEep:TIME 0.5 SECS

-138 Suffix not allowed

A suffix was used where none were expected. Example: Using a suffix when not allowed.

SOURce1:BURSt: NCYCles 12 CYC

-148 Character data not allowed

A parameter was used in the command where not allowed. Example: A discrete parameter was used where a numeric parameter was expected.

SOUR1:MARK:FREQ ON

-158 String data not allowed

An unexpected character string was used where none were expected. Example: A character string is used instead of a valid parameter.

SOURce1:SWEep:SPACing 'TEN'

-161 Invalid block data

Invalid block data was received. Example: The number of bytes sent with the SOURce[1|2]:DATA:DAC command doesn't correlate to the number of bytes specified in the block header.

-168 Block data not allowed

Block data was received where block data is not allowed. Example:

SOURce1:BURSt: NCYCles #10

-170~178 expression errors

Example: The mathematical expression used was not valid.

Execution Errors

-211 Settings conflict;infinite burst changed trigger source to MANual

Example: The trigger source is changed to Immediate from manual when infinite burst mode is selected.

-223 Settings conflict;frequency forced duty cycle change

Example: If the frequency is changed and the current Duty cannot be supported at the new frequency ,the Duty will be automatically adjusted.

-221 Settings conflict; frequency reduced for ramp function

Example: When the function is changed to ramp,the Output frequency is automatically reduced if over range.

-221 Settings conflict; when amplitude coupling,the other channel can't be set to "power"units

Example: The dBm units can not be used when amplitude coupling, the other channel uses high_z load

-221 Settings conflict; coupling has forced tracking off.

Example: When coupling mode is enabled,tracking mode is automatically disabled.

-221 Settings conflict;trace mode doesn't support ARB

Example: When ARB mode is enabled,tracking mode is automatically disabled.

-221 Settings conflict;The phase function doesn't support ARB,square wave pulse waveforms.

Example:The phase function doesn't support ARB.

-221 Settings conflict;Burst function can not be performed under current setting

Example: A burst waveform cannot be generated with the noise or pulse waveforms.

-221 Settings conflict;Sweep function can not be performed under current setting.

Example: A sweep waveform cannot be generated with the noise or pulse waveforms.

-221 Settings conflict;Noise and ARB don't support frequency coupling

Example: The frequency coupling waveform can not be generated with the noise or ARB waveforms.

-221 Settings conflict;Arb doesn't support phase operation in burst mode.

Example: When burst mode is enabled,the parameter of phase can not be change.

-221 Settings conflict;Sweep mode doesn't support frequency coupling

Example:When modulation mode is enabled,amplitude coupling mode is automatically disabled.

-221 Settings conflict;Burst mode doesn't support frequency coupling.

Example: When burst mode is enabled,amplitude coupling mode is automatically disabled.

-221 Settings conflict;Modulation mode doesn't support frequency coupling.

Example: When modulation is enabled,frequency coupling is automatically disabled.

-221 Settings conflict;Tracking has forced coupling off.

Example: When tracking mode is enabled,coupling mode is automatically disabled.

-221 Settings conflict; Coupling can not be performed under current setting

Example: When sweep mode is enabled,coupling mode is automatically disabled.

-221 Settings conflict;The dBm units can not used,when load is high_z.

Example: The dBm units can not be used when the load is high_z.

-221 Settings conflict;value clipped to upper limit.

Example: The parameter was set out of range. The parameter is automatically set to the maximum value allowed.

-221 Settings conflict;modulation function can not be performed under current setting.

Example: A modulated waveform cannot be generated with the noise or pulse waveforms.

-222 Data out of range;value clipped to lower limit

Example: The parameter was set out of range.The parameter is automatically set to the minimum value allowed.

-222 Data out of range;amplitude

Example: If the amplitude was set to a value out of range ,it is automatically set to an upper or lower limit.

-222 Data out of range;offset

Example: If the offset is set to a value out of range,it is automatically set to an upper of lower limit.

-222 Data out of range;burst count

Example: If the burst count was set to a value out of range, it is automatically set to an upper or lower limit.

-222 Data out of range;FM deviation clipped to upper limit

Example: If the FM dev was set to a value out of range, it is automatically set to an upper or lower limit.

-222 Data out of range;Pulse width limited by period

Example: If the width was set to a value out of range,it is automatically set to an upper or lower limit.

-222 Data out of range;frequency

Example: If the frequency was set to a value out of range,it is automatically set to an upper or lower limit.

Query Errors

-410 Query INTERRUPTED

Indicates that a command was received but the data in the output buffer from a previous command was lost.

-420 Query UNTERMINATED

The function generator is ready to return data, however there was no data in the output buffer. For example: Using the APPLy command.

-430 Query DEADLOCKED

Indicates that a command generates more data than the output buffer can receive and the input buffer is full. The command will finish execution, though all the data won't be kept.

Arbitrary Waveform Errors

-770 Nonvolatile arb waveform memory corruption detected

Indicates that a fault (check sum error) has occurred with the non-volatile memory that stores the arbitrary waveform data.

-781 Not enough memory to store new arb waveform; bad sectors

Indicates that a fault (bad sectors) has occurred with the non-volatile memory that stores the arbitrary waveform data. Resulting in not enough memory to store arbitrary data.

-787 Not able to delete the currently selected active arb waveform

Example: The currently selected waveform is being output and cannot be deleted.

800 Block length must be even

Example: As block data (SOURce[1|2]:DATA:DAC VOLATILE) uses two bytes to store each data point, there must be an even number or bytes for a data block.

SCPI Status Register

The status registers are used to record and determine the status of the function generator.

The function generator has a number of register groups:

Questionable Status Registers

Standard Event Status Registers

Status Byte Register

As well as the output and error queues.

Each register group is divided into three types of registers: condition registers, event registers and enable registers.

Register types

Condition Register	The condition registers indicate the state of the function generator in real time. The condition registers are not triggered. I.e., the bits in the condition register change in real time with the instrument status. Reading a condition register will not clear it. The condition registers cannot be cleared or set.
Event Register	The Event Registers indicate if an event has been triggered in the condition registers. The event registers are latched and will remain set unless the *CLS command is used. Reading an event register will not clear it.
Enable Register	The Enable register determines which status event(s) are enabled. Any status events that are not enabled are ignored. Enabled events are used to summarize the status of that register group.

AFG-2225 Status System

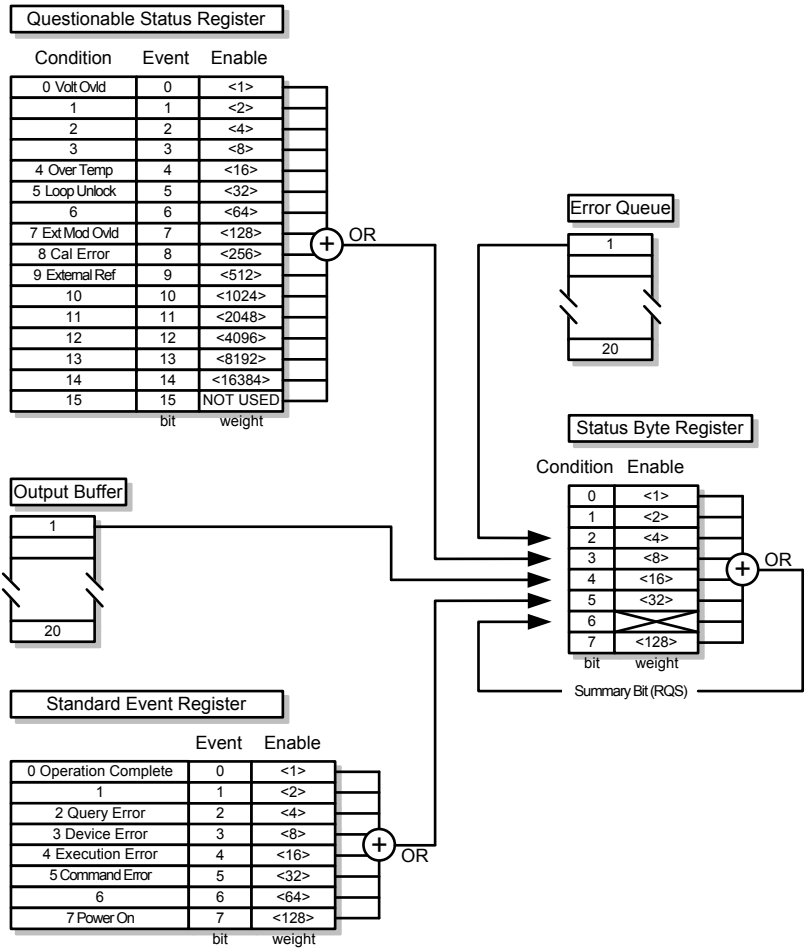

Questionable Status Register

Description: The Questionable Status Registers will show if any faults or errors have occurred.

Bit Summary

Register	Bit	Bit Weight
Voltage overload	0	1
Over temperature	4	16
Loop unlock	5	32
Ext Mod Overload	7	128
Cal Error	8	256
External Reference	9	512

Standard Event Status Registers

Description: The Standard Event Status Registers indicate when the *OPC command has been executed or whether any programming errors have occurred.

Notes: The Standard Event Status Enable register is cleared when the *ESE 0 command is used.

The Standard Event Status Event register is cleared when the *CLS command or the *ESR? command is used.

Bit Summary	Register	Bit	Bit Weight
	Operation complete bit	0	1
	Query Error	2	4
	Device Error	3	8
	Execution Error	4	16
	Command Error	5	32
	Power On	7	128

Error Bits		
	Operation complete	The operation complete bit is set when all selected pending operations are complete. This bit is set in response to the *OPC command.
	Query Error	The Query Error bit is set when there is an error reading the Output Queue. This can be caused by trying to read the Output Queue when there is no data present.
	Device Error	The Device Dependent Error indicates a failure of the self-test, calibration, memory or other device dependent error.
	Execution Error	The Execution bit indicates an execution error has occurred.
	Command Error	The Command Error bit is set when a syntax error has occurred.
	Power On	Power has been reset.

The Status Byte Register

Description

The Status Byte register consolidates the status events of all the status registers. The Status Byte register can be read with the *STB? query or a serial poll and can be cleared with the *CLS command.

Clearing the events in any of the status registers will clear the corresponding bit in the Status Byte register.

Notes

The Status byte enable register is cleared when the *SRE 0 command is used.

The Status Byte Condition register is cleared when the *CLS command is used.

Bit Summary

Register	Bit	Bit Weight
Error Queue	2	4
Questionable Data	3	8
Message Available	4	16
Standard Event	5	32
Master Summary / Request Service	6	64

Status Bits

Error Queue	There are error message(s) waiting in the error queue.
Questionable data	The Questionable bit is set when an “enabled” questionable event has occurred.
Message Available	The Message Available bit is set when there is outstanding data in the Output Queue. Reading all messages in the output queue will clear the message available bit.

	Standard Event	The Event Status bit is set if an "enabled" event in the Standard Event Status Event Register has occurred.
	Master Summary/ Service Request bit	The Master Summary Status is used with the *STB? query. When the *STB? query is read the MSS bit is not cleared. The Request Service bit is cleared when it is polled during a serial poll.

Output Queue

Description	The Output queue stores output messages in a FIFO buffer until read. If the Output Queue has data, the MAV bit in the Status Byte Register is set.

Error Queue

Description	The error queue is queried using the SYSTem:ERRor? command. The Error queue will set the "Error Queue" bit in the status byte register if there are any error messages in the error queue. If the error queue is full the last message will generate a "Queue overflow" error and additional errors will not be stored. If the error queue is empty, "No error" will be returned. Error messages are stored in the error queue in a first-in-first-out order. The errors messages are character strings that can contain up to 255 characters.

APPENDIX

AFG-2225 Specifications

The specifications apply when the function generator is powered on for at least 30 minutes under +18°C~+28°C.

AFG-2225 models		CH1	CH2
Waveforms		Sine, Square, Ramp, Pulse, Noise, ARB	
Arbitrary Functions(1)			
	Sample Rate	120 MSa/s	
	Repetition Rate	60MHz	
	Waveform Length	4k points	
	Amplitude Resolution	10 bits	
	Non-Volatile Memory	4k points	
Frequency Characteristics			
Range	Sine	1uHz~25MHz	
	Square	1uHz~25MHz	
	Ramp	1MHz	
Resolution		1uHz	
Accuracy	Stability	±20 ppm	
	Aging	±1 ppm, per 1 year	
	Tolerance	≤1 mHz	
Output Characteristics			
Amplitude	Range	1mVpp to 10 Vpp (into 50Ω) 2mVpp to 20 Vpp (open-circuit) 1mVpp to 5 Vpp (into 50Ω) for 20MHz-25MHz 2mVpp to 10 Vpp (open-circuit) for 20MHz-25MHz	
	Accuracy	±2% of setting ±1 mVpp (at 1 kHz)	
	Resolution	1mV or 3 digits	
	Flatness	±1% (0.1dB) ≤100kHz ±3% (0.3 dB) ≤5MHz ±5% (0.4 dB) ≤12MHz ±10%(0.9dB) ≤25MHz (sine wave relative to 1kHz)	
	Units	Vpp, Vrms, dBm	

Offset	Range	±5 Vpk ac +dc (into 50Ω) ±10Vpk ac +dc (Open circuit) ±2.5 Vpk ac +dc (into 50Ω) for 20MHz-25MHz ±5Vpk ac +dc (Open circuit) for 20MHz-25MHz	
	Accuracy	2% of setting + 10mV+ 0.5% of amplitude	
Waveform Output	Impedance	50Ω typical (fixed) > 10MΩ (output disabled)	
	Protection	Short-circuit protected Overload relay automatically disables main output	
Sine wave Characteristics			
	Harmonic distortion	≤-55 dBc DC ~ 200kHz, Ampl > 0.1Vpp ≤-50 dBc 200kHz ~ 1MHz, Ampl > 0.1Vpp ≤-35 dBc 1MHz ~ 5MHz, Ampl > 0.1Vpp ≤-30 dBc 5MHz ~ 25MHz, Ampl > 0.1Vpp	
Square wave Characteristics			
	Rise/Fall Time	≤25ns at maximum output. (into 50 Ω load)	
	Overshoot	5%	
	Asymmetry	1% of period +5 ns	
	Variable duty Cycle	1.0% to 99.0% ≤100kHz 10% to 90% ≤ 1MHz 50% ≤ 25MHz	
Ramp Characteristics			
	Linearity	< 0.1% of peak output	
	Variable Symmetry	0% to 100% (0.1% Resolution)	
Pulse Characteristics			
	Period	40ns~2000s	
	Pulse Width（2）	20ns~1999.9s	
	Overshoot	<5%	
	Accuracy	0.1%+20ns	
	Jitter	20ppm +10ns	
AM Modulation			
	Carrier Waveforms	Sine, Square, Ramp, Pulse,Arb	Sine, Square, Ramp, Pulse,Arb
	Modulating Waveforms	Sine, Square, Triangle, Upramp, Dnramp	Sine, Square, Triangle, Upramp, Dnramp
	Modulating Frequency	2mHz to 20kHz (Int) DC to 20kHz (Ext)	2mHz to 20kHz (Int) DC to 20kHz (Ext)
	Depth	0% to 120.0%	0% to 120.0%
	Source	Internal / External	Internal / External
FM Modulation			
	Carrier Waveforms	Sine, Square, Ramp,	Sine, Square, Ramp,
	Modulating Waveforms	Sine, Square, Triangle, Upramp, Dnramp	Sine, Square, Triangle, Upramp, Dnramp

	Modulating Frequency	2mHz to 20kHz (Int) DC to 20kHz (Ext)	2mHz to 20kHz (Int) DC to 20kHz (Ext)
	Peak Deviation	DC to Max Frequency	DC to Max Frequency
	Source	Internal / External	Internal / External
Sweep			
	Waveforms	Sine, Square, Ramp,	Sine, Square, Ramp,
	Type	Linear or Logarithmic	Linear or Logarithmic
	Start/Stop Freq	1uHz to Max Frequency	1uHz to Max Frequency
	Sweep Time	1ms to 500s	1ms to 500s
	Source	Internal / External/Manual	Internal / External/Manual
FSK			
	Carrier Waveforms	Sine, Square, Ramp,Pulse	Sine, Square, Ramp,Pulse
	Modulating Waveforms	50% duty cycle square	50% duty cycle square
	Modulation Rate	2mHz to 100 kHz (INT) DC to 100 kHz(EXT)	2mHz to 100 kHz (INT) DC to 100 kHz(EXT)
	Frequency Range	1uHz to Max Frequency	1uHz to Max Frequency
	Source	Internal / External	Internal / External
PM			
	Carrier Waveforms	Sine, Square, Ramp	Sine, Square, Ramp
	Modulating Waveforms	Sine, Square, Triangle, Upramp, Dnramp	Sine, Square, Triangle, Upramp, Dnramp
	Modulation Frequency	2mHz to 20kHz (Int) DC to 20kHz (Ext)	2mHz to 20kHz (Int) DC to 20kHz (Ext)
	Phase deviation	0° to 360°	0° to 360°
	Source	Internal / External	Internal / External
SUM			
	Carrier Waveforms	Sine, Square, Ramp,Pulse,Noise	Sine, Square, Ramp,Pulse,Noise
	Modulating Waveforms	Sine, Square, Triangle, Upramp,Dnramp	Sine, Square, Triangle, Upramp,Dnramp
	Modulation Frequency	2mHz to 20kHz (Int) DC to 20kHz (Ext)	2mHz to 20kHz (Int) DC to 20kHz (Ext)
	SUM Depth	0% to 100.0%	0% to 100.0%
	Source	Internal / External	Internal / External
External Trigger Input			
	Type	For FSK, Burst, Sweep	
	Input Level	TTL Compatibility	
	Slope	Rising or Falling(Selectable)	
	Pulse Width	>100ns	
	Input Impedance	10kΩ，DC coupled	

External Modulation Input			
	Type	For AM, FM, PM, SUM	
	Voltage Range	±5V full scale	
	Input Impedance	10kΩ	
	Frequency	DC to 20kHz	
Trigger Output			
	Type	For Burst, Sweep, Arb	
	Level	TTL Compatible into 50Ω	
	Pulse Width	>450ns	
	Maximum Rate	1MHz	
	Fan-out	≥4 TTL Load	
	Impedance	50Ω Typical	
Dual Channel Function			
	Phase（3）	-180° ~180°	-180° ~ 180°
		Synchronize phase	Synchronize phase
	Track	CH2=CH1	CH1=CH2
	Coupling	Frequency(Ratio or Difference)	Frequency(Ratio or Difference)
		Amplitude & DC Offset	Amplitude & DC Offset
	Dsolink	√	√
Burst			
	Waveforms	Sine, Squa, Ramp,Arb	Sine, Squa,Ramp,Arb
	Frequency（4）	1uHz~15 MHz	1uHz~15 MHz
	Burst Count	1 to 65535 cycles or Infinite	1 to 65535 cycles or Infinite
	Start/Stop Phase	-360 to +360	-360 to +360
	Internal Period	1ms to 500s	1ms to 500s
	Gate Source	External Trigger	External Trigger
	Trigger Source	Single, External or Internal Rate	Single, External or Internal Rate
Trigger Delay	N-Cycle, Infinite	0s to 655350ns	0s to 655350ns
Frequency Counter			
	Range	5Hz to 150MHz	
	Accuracy	Time Base accuracy±1count	
	Time Base	±20ppm (23°C ±5°C) after 30 minutes warm up	
	Resolution	The maximum resolution is: 100nHz for 1Hz, 0.1Hz for 100MHz.	
	Input Impedance	1kΩ/1pf	
	Sensitivity	35mVrms ~ 30Vms (5Hz to 150MHz)	
Save/Recall		10 Groups of Setting Memories	
Interface		USB (Host&Device)	
Display		TFT	
General Specifications			
	Power Source	AC100~240V, 50~60Hz	
	Power Consumption	25 W (Max)	

Operating Environment	Temperature to satisfy the specification : 18 ~ 28˚C Operating temperature : 0 ~ 40˚C Relative Humidity: < 80%, 0 ~ 40˚C Installation category : CAT II
Operating Altitude	2000 Meters
Storage Temperature	-10~70˚C, Humidity: ≤70%
Dimensions (WxHxD)	266(W) x 107(H) x 293(D) mm
Weight	Approx. 2.5kg
Accessories	GTL-101× 2 Quick Start Guide ×1 CD (user manual + software) ×1 Power cord×1

(1) Filter bandwidth 20MHz -3Db.

(2) Pulse amplitude will decrease when pulse width is <50ns

(3) Square and Pulse can not be change, Phase is 0°

(4)

1uHz~15 MHz(Sine)	1uHz~15 MHz(Sine)
1uHz~15 MHz (Squa)	1uHz~15 MHz (Squa)
1uHz~1 MHz (Ramp)	1uHz~1 MHz (Ramp)

EC Declaration of Conformity

We

GOOD WILL INSTRUMENT CO., LTD.

No.7-1, Jhongsing Rd., Tucheng Dist., New Taipei City 236, Taiwan

GOOD WILL INSTRUMENT (SUZHOU) CO., LTD.

No. 69, Lushan Road, Suzhou New District Jiangsu, China

declares that the below mentioned product

AFG-2225

Are herewith confirmed to comply with the requirements set out in the Council Directive on the Approximation of the Law of Member States relating to Electromagnetic Compatibility (2004/108/EC) and Low Voltage Equipment Directive (2006/95/EC). For the evaluation regarding the Electromagnetic Compatibility and Low Voltage Equipment Directive, the following standards were applied:

◎ **EMC**

EN 61326-1: EN 61326-2-1:	**Electrical equipment for measurement, control and laboratory use — EMC requirements (2006)**
Conducted and Radiated Emissions EN 55011: 2009+A1:2010 （Class A)	Electrostatic Discharge IEC 61000-4-2: 2008
Current Harmonic EN 61000-3-2: 2006+A2:2009	Radiated Immunity IEC 61000-4-3: 2010
Voltage Fluctuation EN 61000-3-3: 2008	Electrical Fast Transients IEC 61000-4-4: 2012
----------	Surge Immunity IEC 61000-4-5: 2005
----------	Conducted Susceptibility IEC 61000-4-6: 2008
----------	Power Frequency Magnetic Field IEC 61000-4-8: 2009
----------	Voltage Dips/ Interrupts IEC 61000-4-11: 2004

◎ **Safety**

Low Voltage Equipment Directive 2006/95/EC
Safety Requirements **EN 61010-1: 2010**

Commmon

Absatan
y=|atan(x)|
The absolute of atan(x)



Abssin
y=|sin(x)|
The absolute of sin(x)

Abssinehalf
y=sin(x),0<x<pi
y=0,pi<x<2pi
Half_wave function



Ampalt
y=e(x).sin(x)
Oscillation rise



Attalt
y=e(-x).sin(x)
Oscillation down



Diric
Even
f(x)=-1^(x*(n-1)/2*pi)
x=0,±2*pi,±4*pi,……

Diric	Odd f(x)=sin(nx/2)/n*sin(x/2) x=±pi,±3pi，……	
Gauspuls	f(x)=a*e^(-(x-b)^2)/c^2) Gaussian-modulated sinusoidal pulse	
Havercosine	y=(1-sin(x))/2 The havercosine function	
Haversin	y=(1-cos(x))/2 The haversine function	
N_pulse	Negative pulse	
Negramp	y=-x Line segment	

Rectpuls	Sampled aperiodic rectangle



Roundhalf	y=sqrt(1-x^2) The half roud

Sawtoot	Sawtooth or triangle wave



Sinetra	Piecewise function



Sinever	Piecewise function



Stair_down	Step down



Stair_ud	Step up and step down



Stair_up	Step up



Stepresp	Heaviside step function



Traperia	Piecewise function

Tripuls	Sampled aperiodic triangle



Math

Arccos The basic trigonometric function

Arccot The basic trigonometric function



Arccsc The basic trigonometric function



Arcsec The basic trigonometric function



Arcsin The basic trigonometric function



Arcsinh The basic trigonometric function



Arctan	The basic trigonometric function	
Arctanh	The basic trigonometric function	
Cosh	The basic trigonometric function	
Cot	The basic trigonometric function	
Csc	The basic trigonometric function	
Dlorentz	The derivative of the lorentz function . y=-2x/(k*x^2+1)	

Expofall	The exponential decay



Exporise	The exponential rise



Gauss	A waveform representing a gaussian bell curve



Ln	The logarithm function

Lorentz	The derivative of the lorentz function y=1/(k*x^2+1)



Sec	The basic trigonometric function



Sech	The basic trigonometric function 
Sinec	y=sin(x)/x 
Sinh	The basic trigonometric function
Sqrt	y=sqrt(x)
Tan	The basic trigonometric function 
Tanh	The basic trigonometric function 

Xsquare Parabola

Window

Barthannwin	Modified Bartlett-Hann window



Bartlett	The Bartlett window is very similar to a triangular window as returned by the triang function.



Blackman	The blackman window function



Bohmanwin	The bohman window function



Chebyshev	The chebyshev window function



Flattopwin	The flattopwin window function

Hamming	The hamming window function



Hann	The hann window function



Hanning	The hanning window function



Kaiser	The kaiser window function

Triang	The triang window function



Tukeywin	The tukey window function



Engineer

Airy	The airy function



Bessel	The bessel function



Beta	The beta function



Gamm	The gamma function



Legendre	Associated Legendre functions



Neumann	The neumann function



INDEX

AM commands 218
Amplitude counter 140
Apply commands 200
ARB commands 260
ARB error messages 279
Arbitrary waveforms 147
  display 150
  edit 159
  output 169
  protection 166
  save and load 171
Beeper 137
Burst commands 249
Caution symbol 6
Channel Settings 143
Channel tracking 141
Cleaning the instrument 8
Command error codes 273
Command list 189
Coupling commands 268
Declaration of conformity 292
Default settings 52
Digital inputs
  how to use 23
Display
  diagram 18
Disposal
  symbol 7
Disposal instructions 9
DSO link 146
EN61010
  measurement category 7
  pollution degree 9
Environment
  safety instructions 8
Error messages 273
FM commands 223
Frequency counter 137
Frequency counter commands 266
Frequency coupling 138
Front panel diagram 13
FSK commands 228
Function keys
  key overview 13
Fuse replacement
  safety instruction 8
Ground
  symbol 6
Help menu 25
lin sweep 113
List of features 11
log sweep 113
Menu Tree 44
Modulation 64
  AM 66
    carrier frequency 68
    carrier shape 67
    depth 72
    frequency 70
    shape 69
    source 73
  amplitude 105
  Burst 118
    count 121
    delay 128
    frequency 120
    modes 119
    output 129
    period 123
    phase 125
    trigger 126
  carrier frequency 102
  carrier wave 101
  FM 75
    carrier frequency 77

carrier shape 76
deviation 81
frequency 79
shape 78
source 82
frequency 104
FSK 84
carrier frequency 86
carrier shape 85
hop frequency 87
rate 88
source 90
PM 91
carrier frequency 93
carrier shape 93
deviation 97
frequency 95
shape 94
source 98
source 106
SUM 100
Sweep 108
marker 115
mode 113
span 111
start 109
stop 109
time 114
trigger 117
wave 103
Operation 54
Amplitude 62
Frequency 60
Noise Wave 59
Offset 63
Pulse width 57
Ramp 58
select waveform 55
Sine 55
Square 56
Operation keys
key overview 13
Output commands 206
Output phase 144
Phase commands 267
Phase sync 145
PM commands 232
Power on/off
safety instruction 7
Power up 20
Pulse configuration commands 216
Query Errors 279
Quick reference 21
ARB 37
burst 35
coupling 42
frequency counter 41
modulation 29
selecting a waveform 27
sweep 34
utility 40
Rear panel diagram 16
Remote control 180
interface configuration 181
Remote interface
Error messages 273
functionality check 182
SCPI registers 281
screen lock 182
Syntax 184
terminal connection 182
Save and recall 132
Save and Recall commands 271
SCPI registers 281
Screen lock 182
Secondary System Settings 131
System and Settings 136
Service operation
about disassembly 7
Set output impedance 143
Setting up the instrument 19
software download 182
Specifications 287
Status register commands 196
SUM commands 236
Sweep commands 240
System commands 193
UK power cord 10
Updating Firmware 136
USB
remote control interface 181
Warning symbol 6